




ALGALTOXKIT F

TEST PROCEDURE

1

PREPARATION OF ALGAL CULTURING MEDIUM

- VOLUMETRIC FLASK (1 liter)
- VIALS WITH NUTRIENT STOCK SOLUTIONS A (2 vials), B, C, D
- DISTILLED (or deionized) WATER

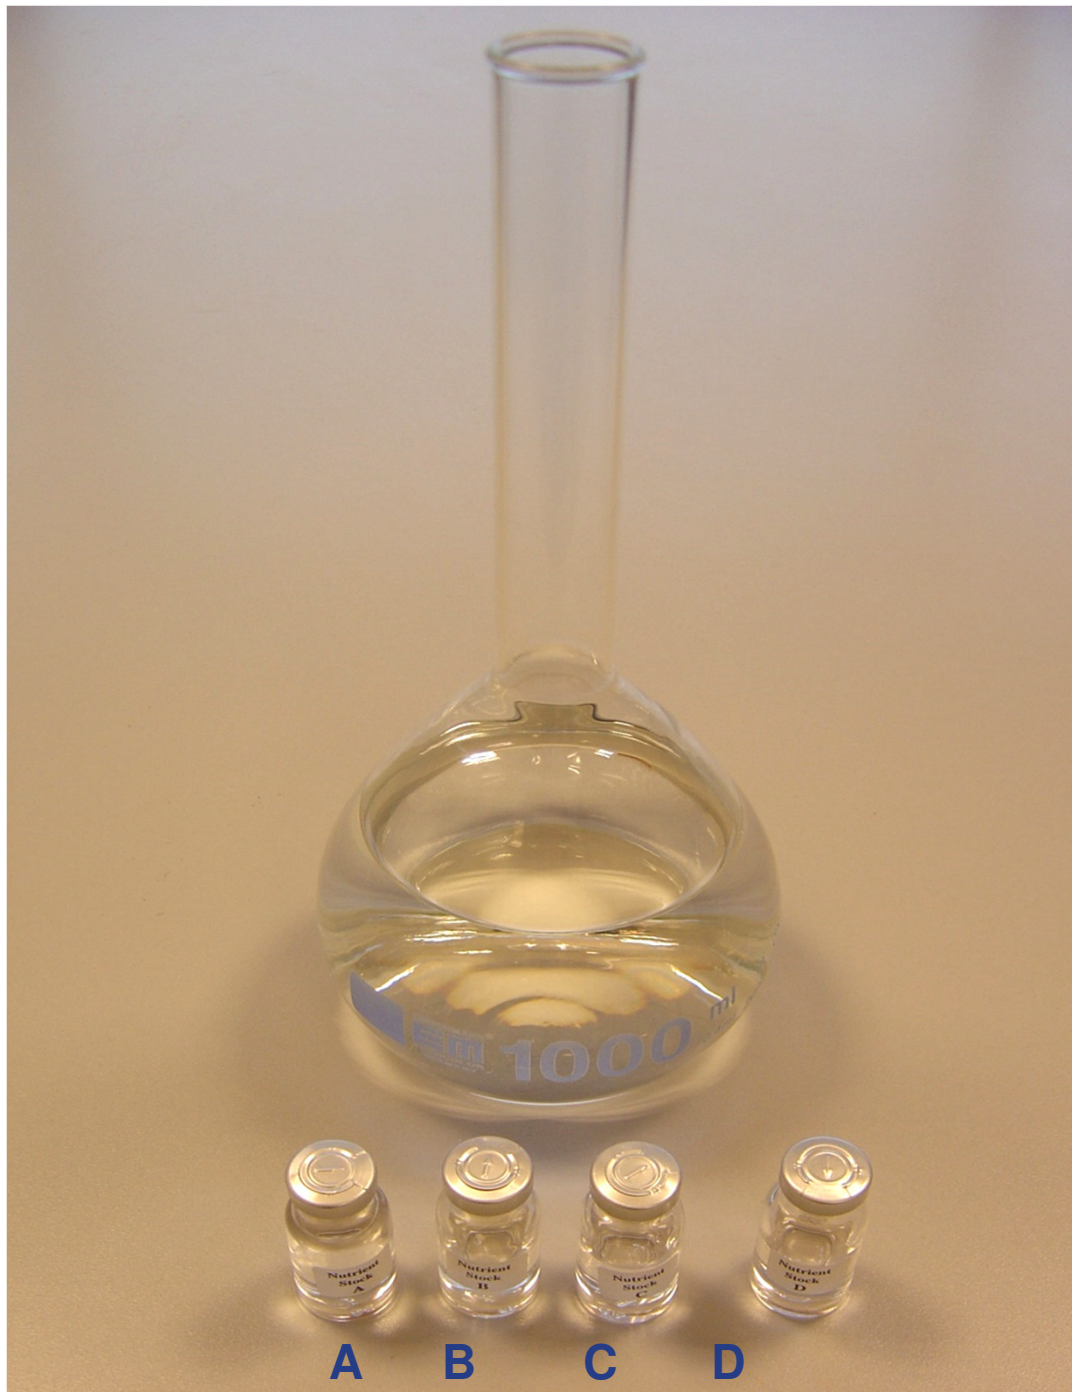

2

**TRANSFER 10 ML FROM ONE OF
THE TWO “NUTRIENT STOCK A” VIALS
IN ± 800 ML DISTILLED WATER
IN THE 1 LITER VOLUMETRIC FLASK**




3

TRANSFER 1 ML FROM THE
NUTRIENT STOCK VIALS
B, C AND D INTO THE 1 LITER
VOLUMETRIC FLASK.




4

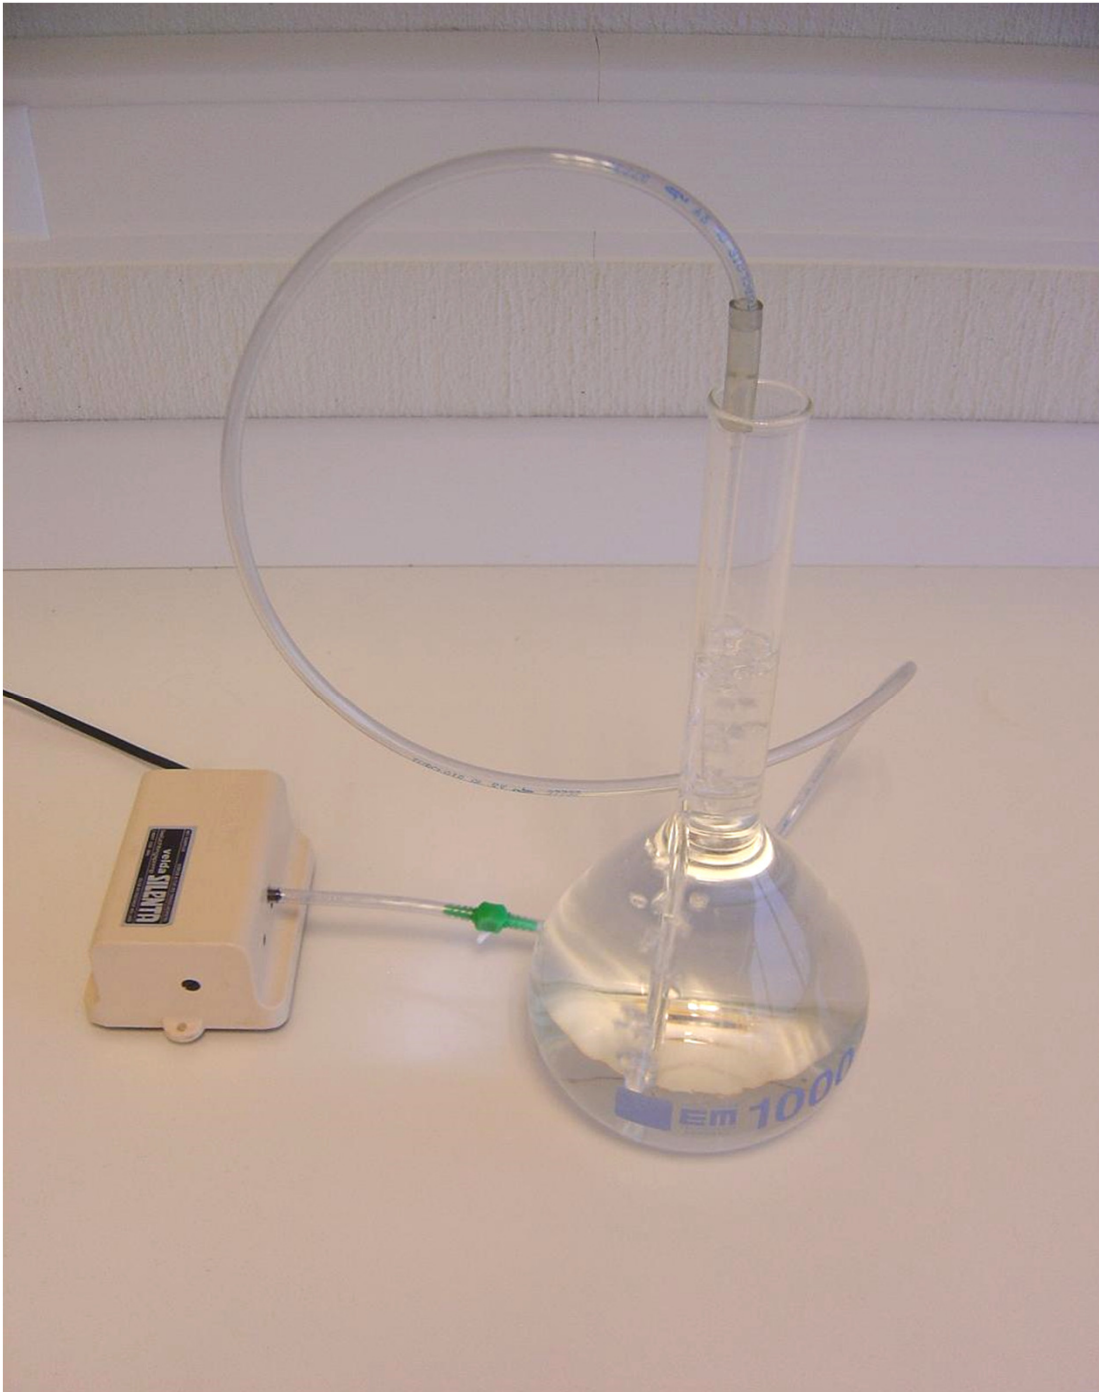


- FILL THE FLASK TO THE 1 LITER MARK WITH DEIONIZED WATER
- STOPPER THE FLASK AND SHAKE THOROUGHLY TO HOMOGENIZE THE CONTENTS
- AERATE THE ALGAL CULTURING MEDIUM FOR AT LEAST 30 MINUTES

5

ADJUST THE pH
(if necessary)
TO $8,1 \pm 0,2$
(with either 1 M HCl
or 1 M NaOH)

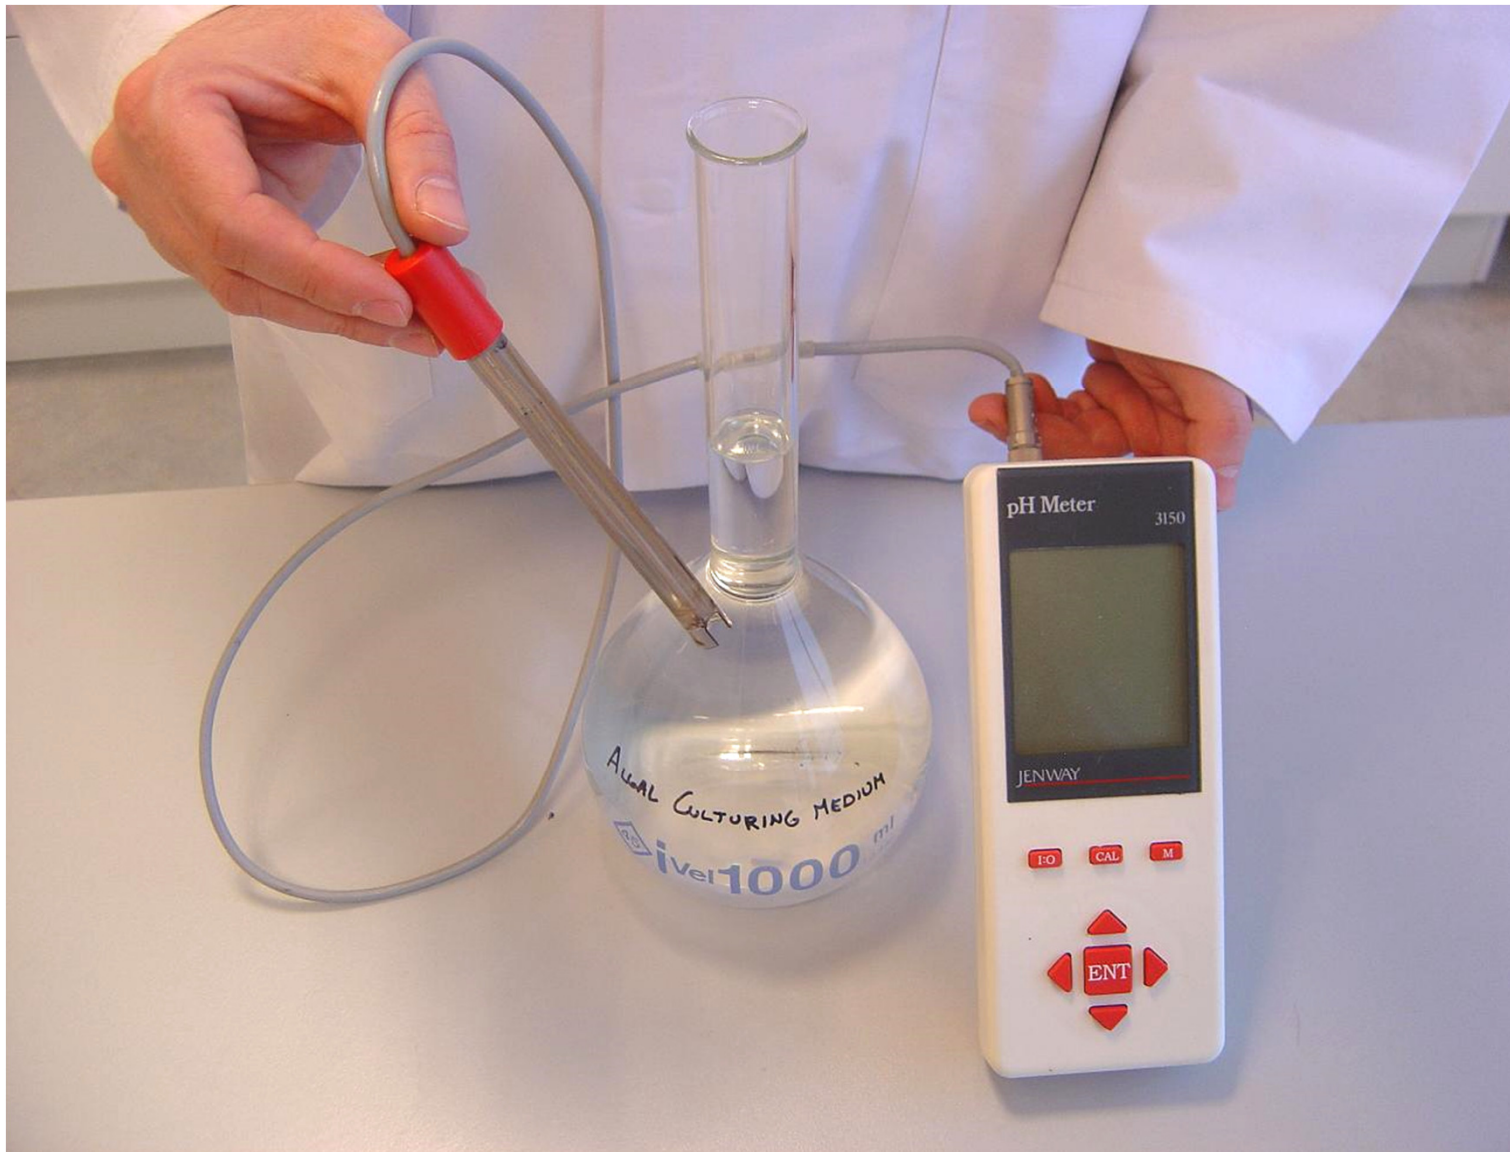

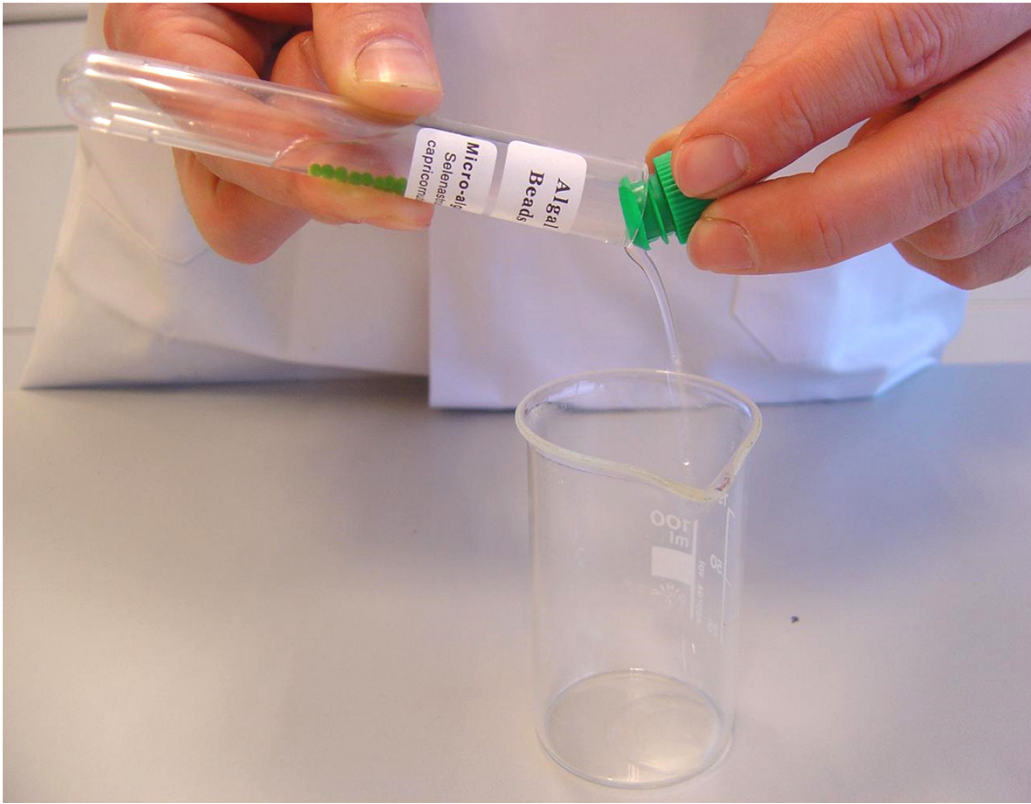

6

DE-IMMOBILISATION OF THE ALGAE

TAKE ONE TUBE CONTAINING ALGAL BEADS AND POUR OUT THE LIQUID
TAKE CARE NOT TO ELIMINATE ANY OF THE ALGAL BEADS DURING THE PROCESS !!



7

OPEN THE VIAL “MATRIX DISSOLVING MEDIUM” AND TRANSFER 5 ML
TO THE TUBE WITH ALGAL BEADS



8

**CAP THE TUBE AND SHAKE VIGOROUSLY TO DISSOLVE THE ALGINATE MATRIX
OF THE ALGAL BEADS, PREFERABLY WITH THE AID OF A VORTEX SHAKER**




9

CONTINUE THE SHAKING UNTIL THE ALGAL BEADS ARE TOTALLY DISSOLVED




10

CENTRIFUGE THE TUBE FOR 10 MINUTES AT 3000 RPM IN A CONVENTIONAL LAB CENTRIFUGE

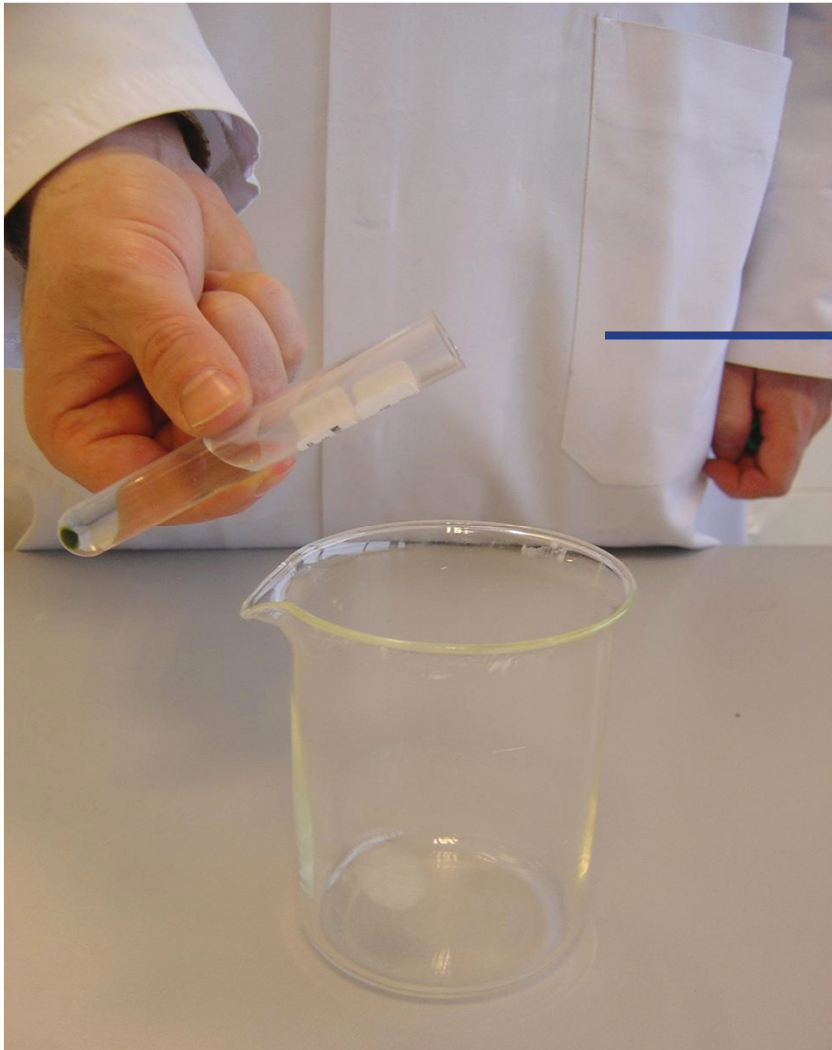


11

POUR OUT THE SUPERNATANT FROM THE TUBE

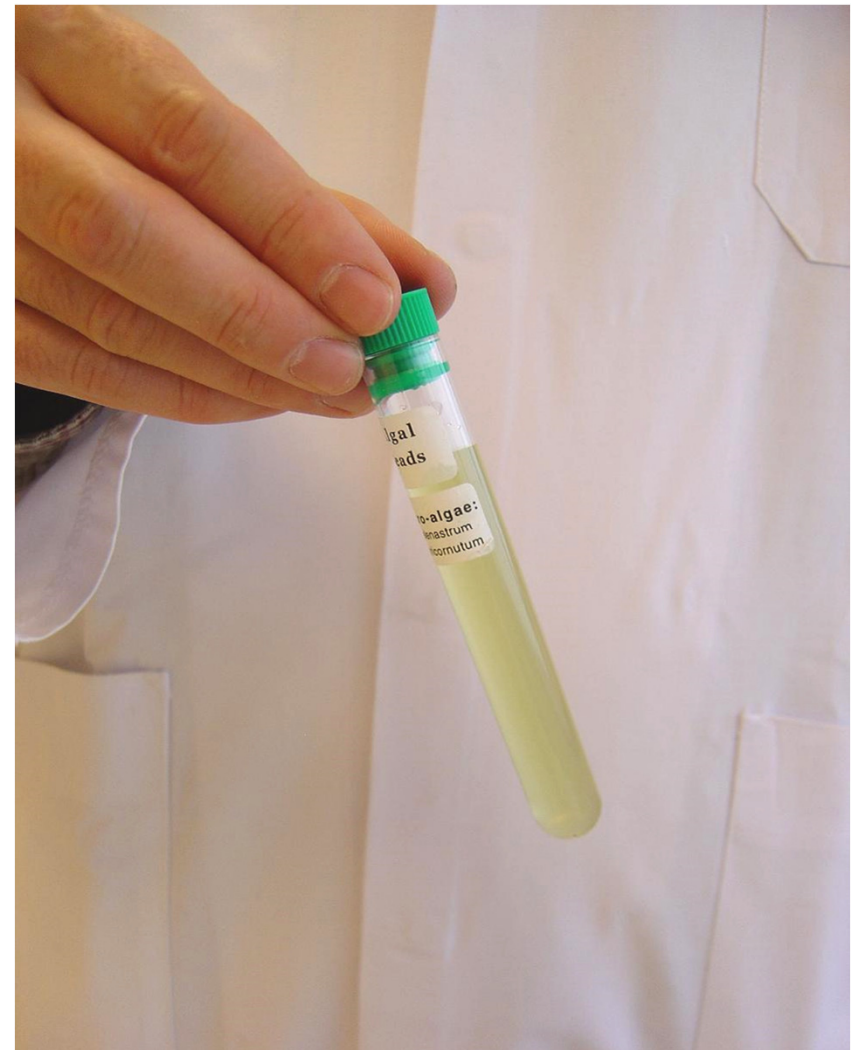

12

- ADD 10 ML DISTILLED WATER TO THE TUBE
- CAP AND SHAKE THE TUBE TO RESUSPEND THE ALGAE

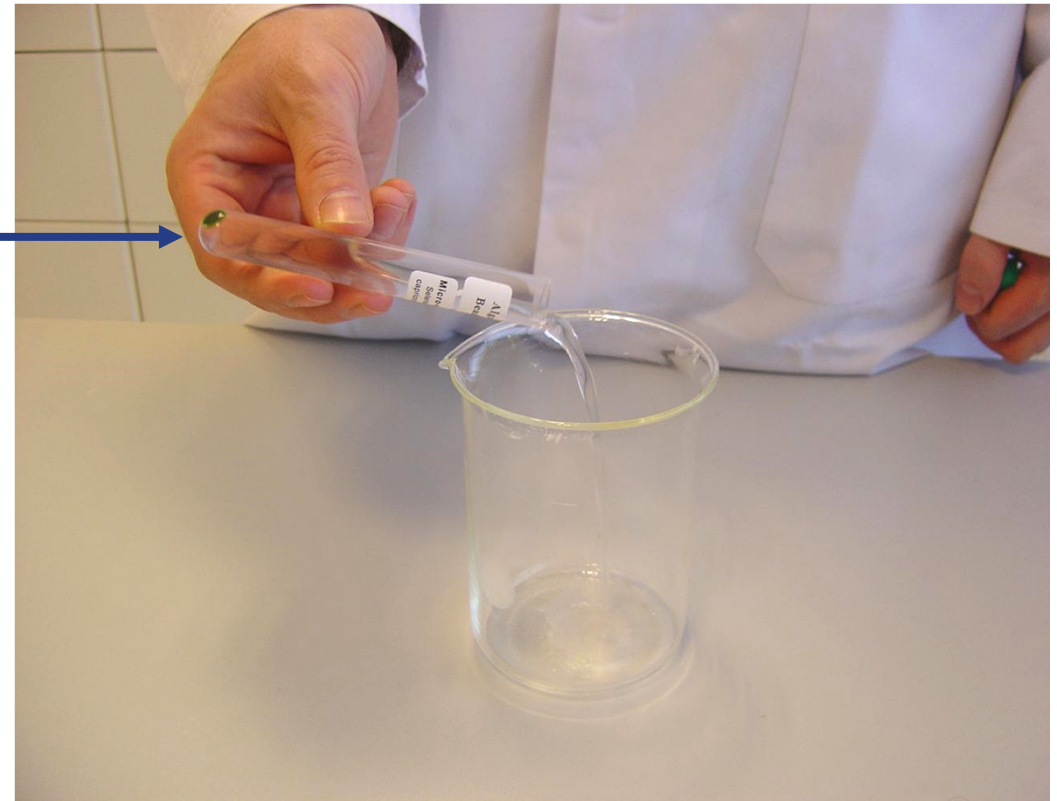


13

CENTRIFUGE THE TUBE AGAIN AT 3000 RPM FOR 10 MINUTES
AND THEN POUR OUT THE SUPERNATANT

14



- ADD 10 ML ALGAL CULTURING MEDIUM TO THE TUBE
- CAP THE TUBE AND SHAKE TO RESUSPEND THE ALGAE

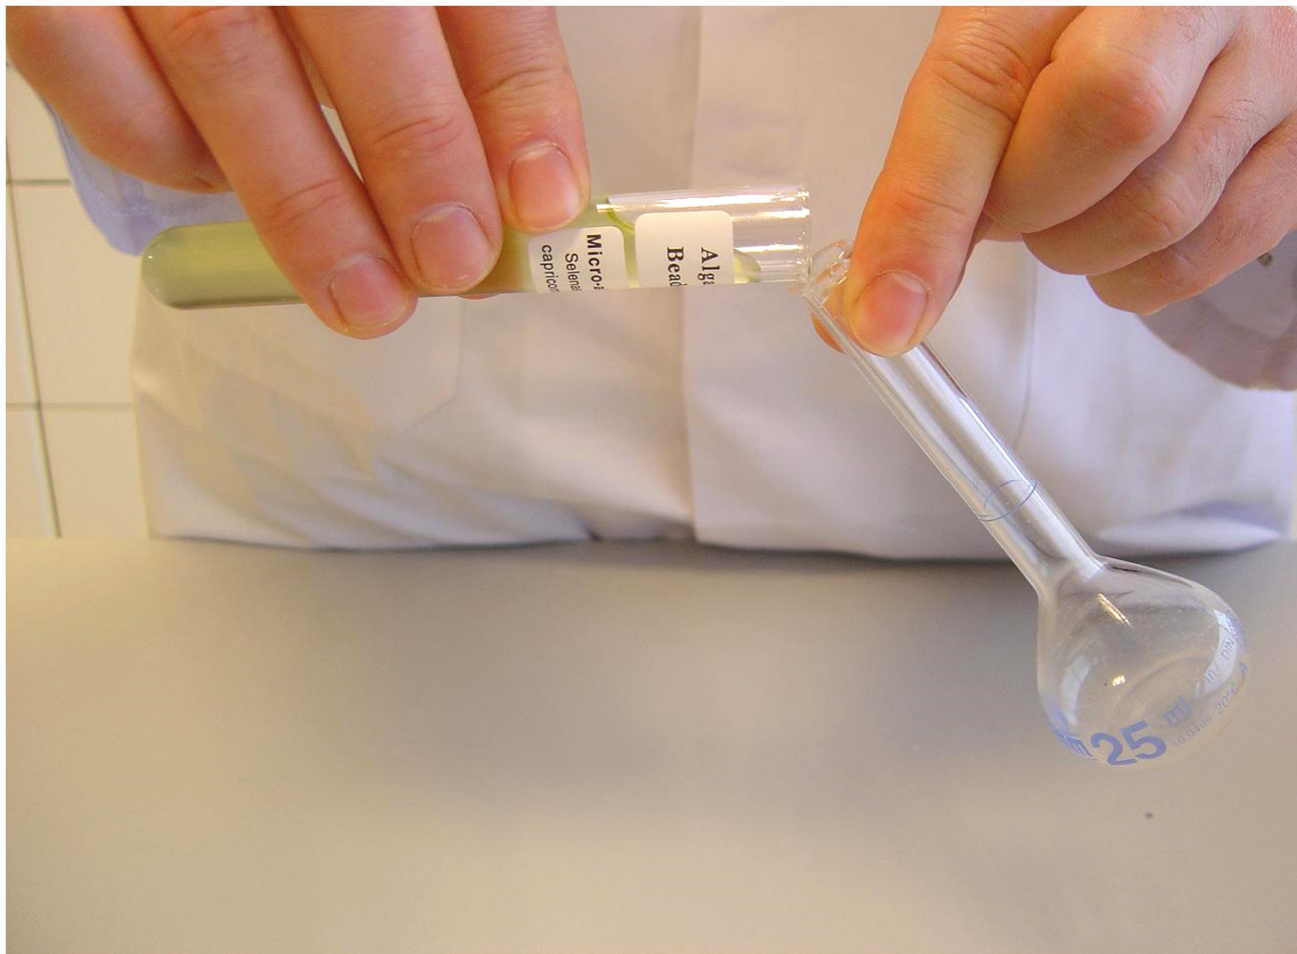

15


PREPARATION OF CONCENTRATED ALGAL INOCULUM

TRANSFER THE ALGAL SUSPENSION FROM THE TUBE INTO A 25 ML CALIBRATED FLASK





16

- ADD ALGAL CULTURING MEDIUM TO THE 25 ML MARK OF THE FLASK
- STOPPER THE FLASK AND SHAKE TO HOMOGENIZE THE ALGAL SUSPENSION

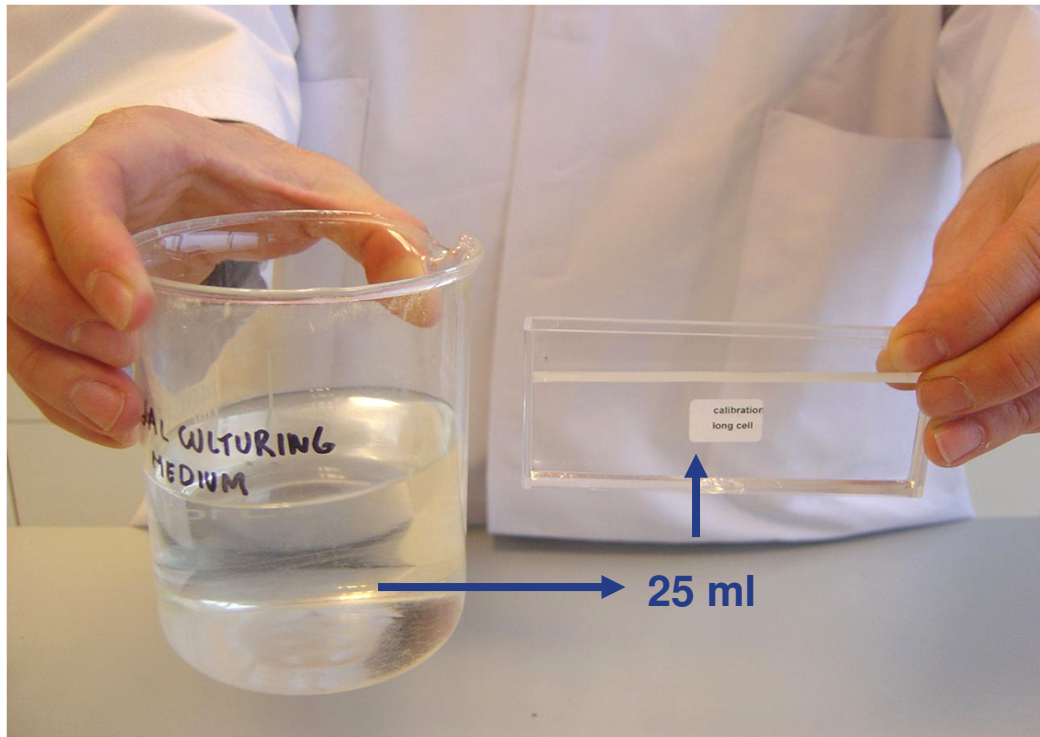


17

- PUT 25 ML ALGAL CULTURING MEDIUM IN THE CALIBRATION LONG CELL AND CLOSE THE CELL WITH THE LID
- PLACE THE CELL IN THE SPECTROPHOTOMETER

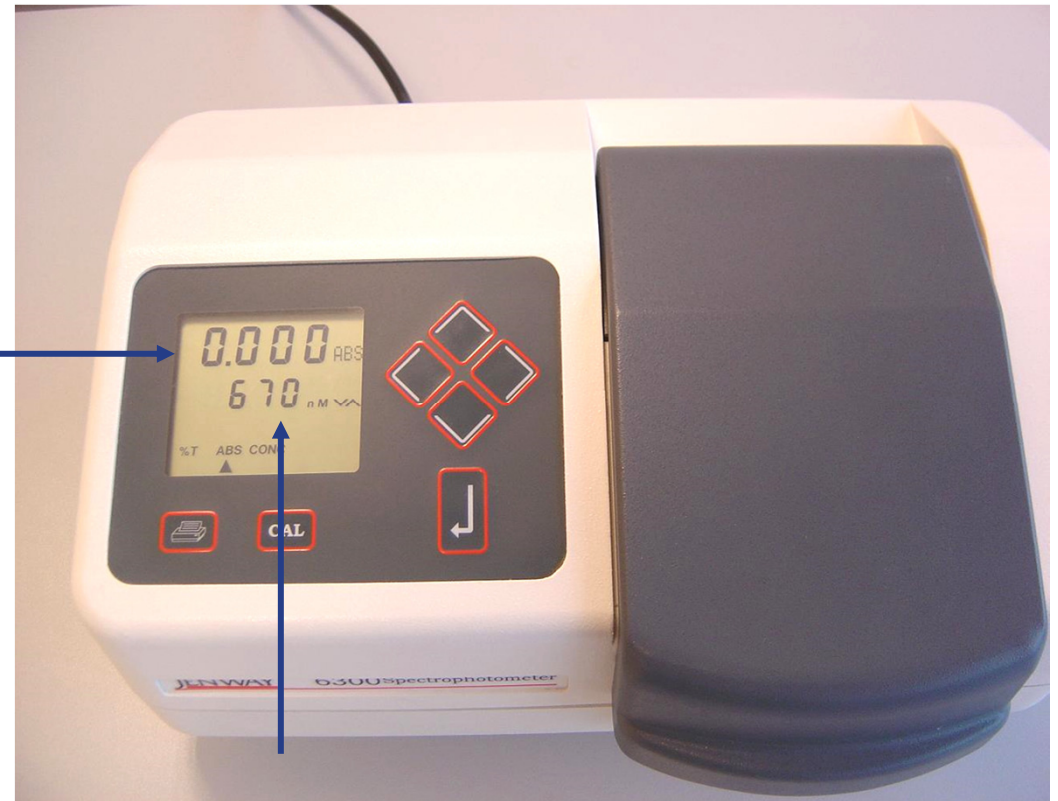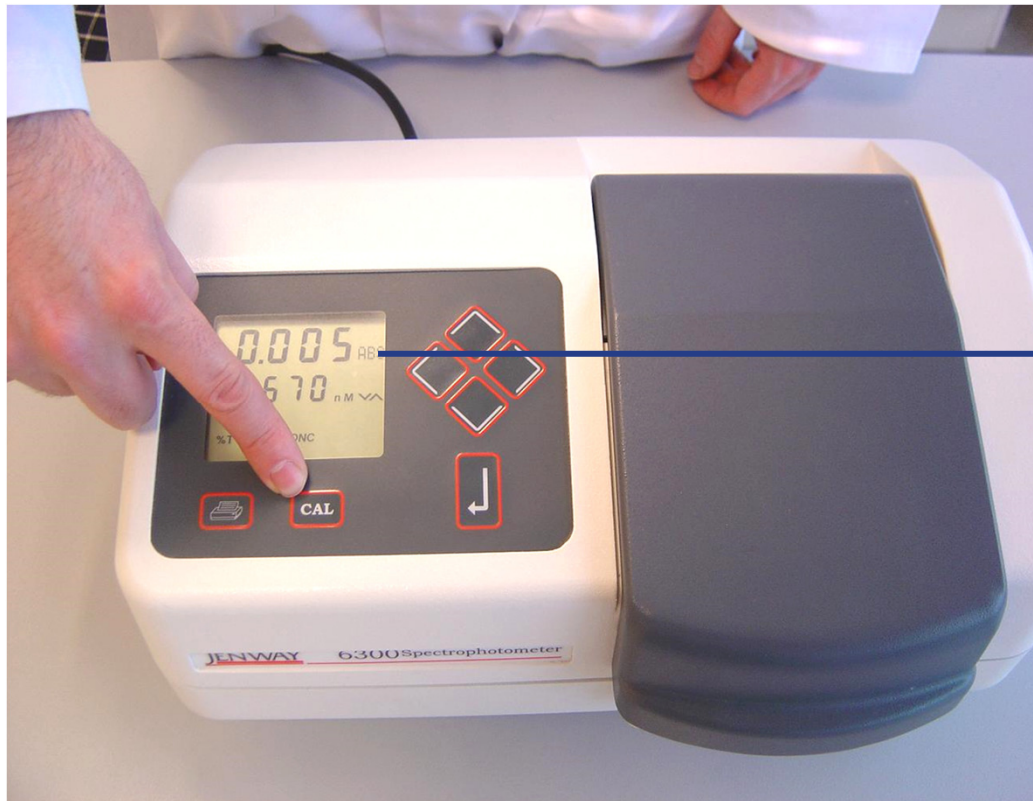


18

ZERO-CALIBRATE THE INSTRUMENT AT A WAVELENGTH OF 670 NM

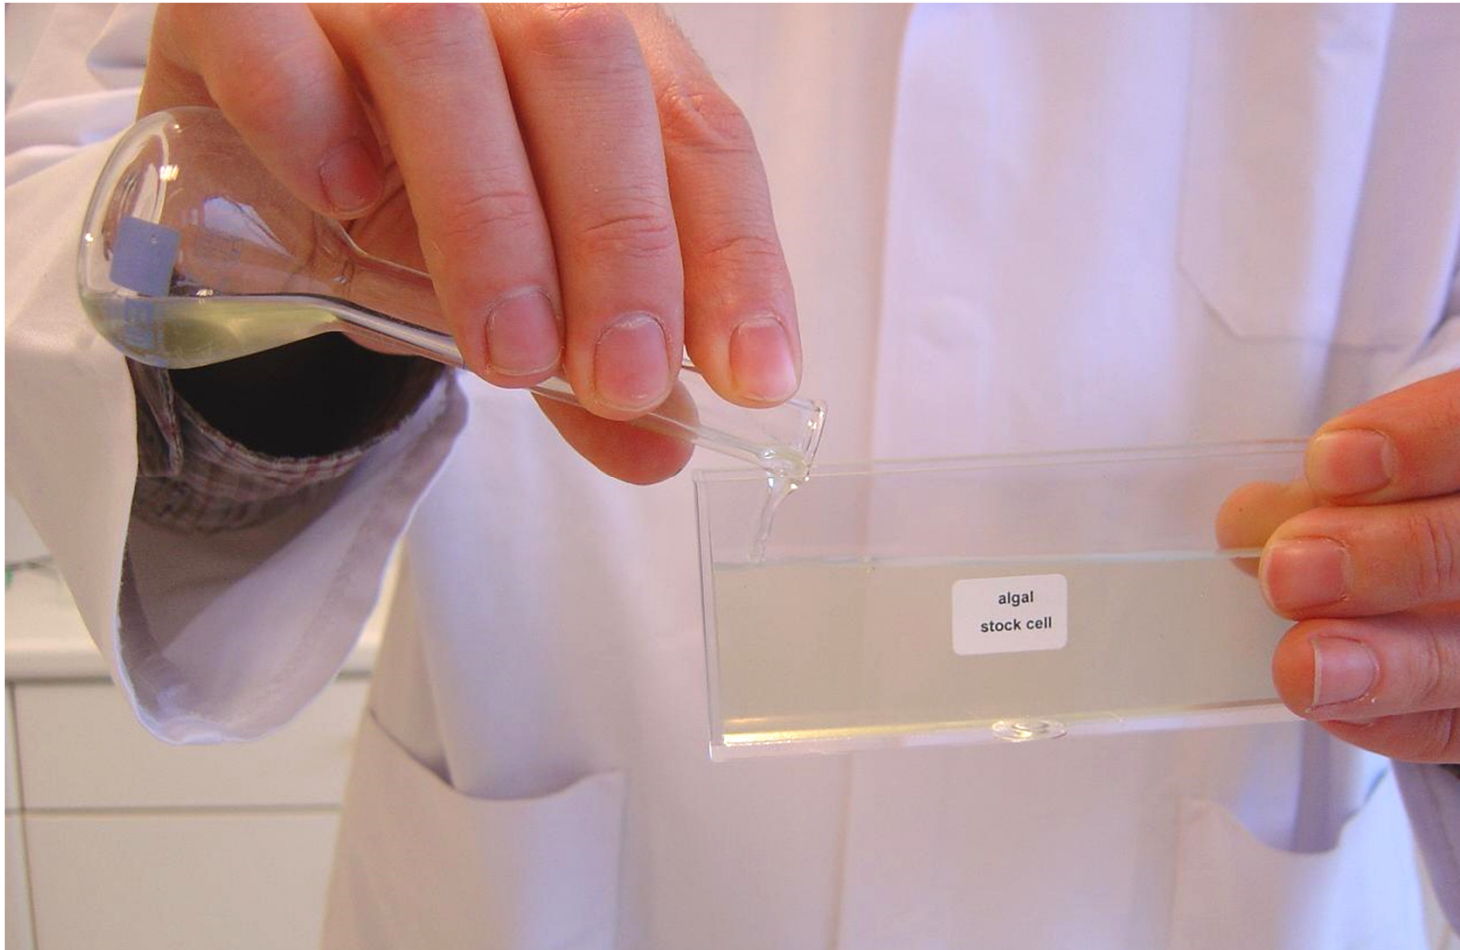


19

TRANSFER THE 25 ML ALGAL SUSPENSION INTO THE ALGAL STOCK CELL

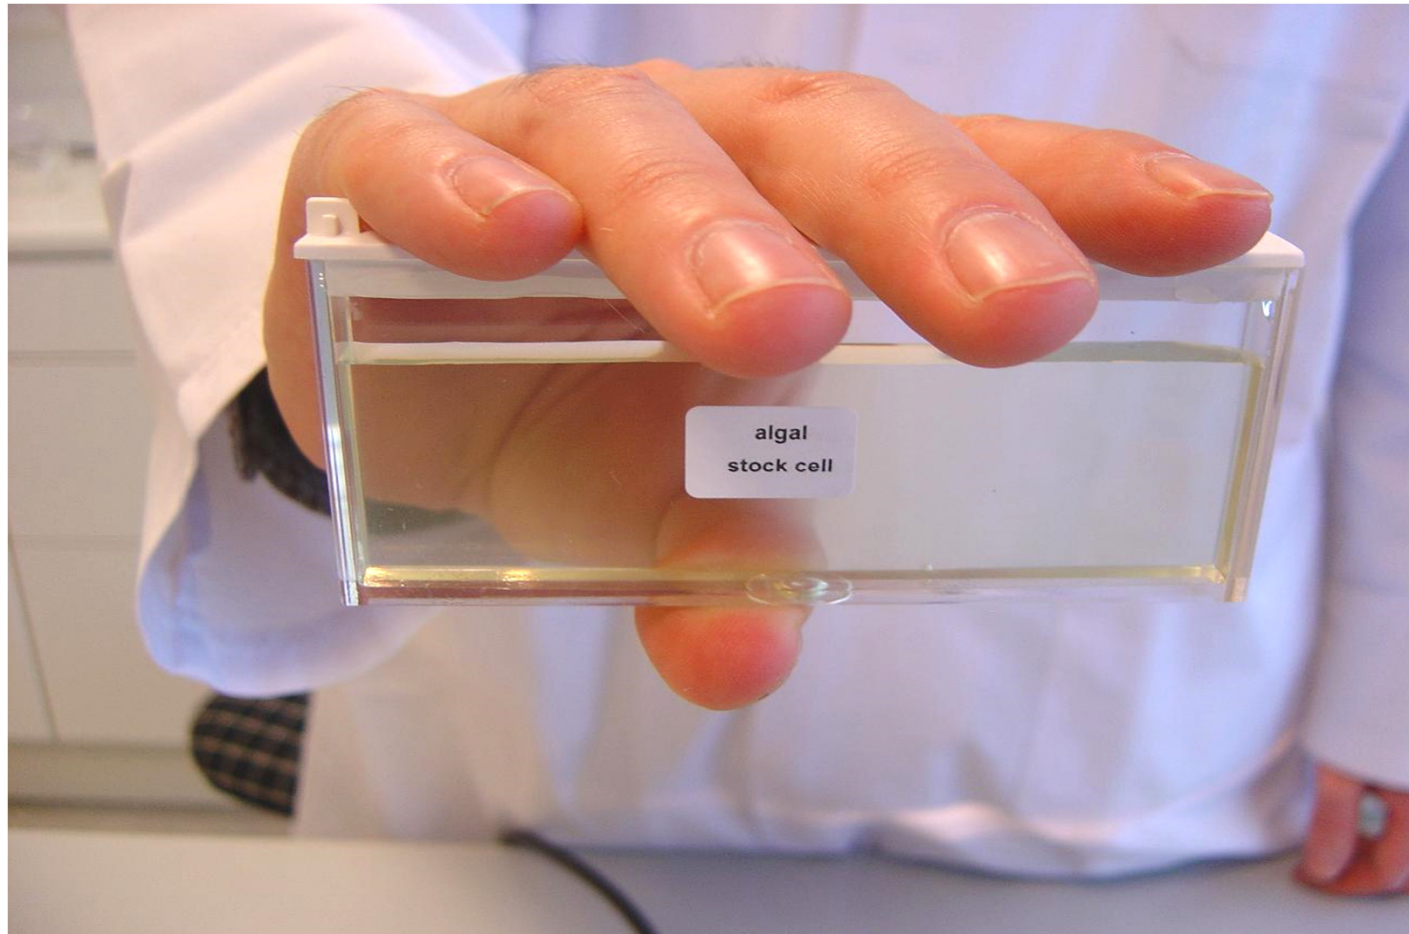


20

**CLOSE THE ALGAL STOCK CELL WITH THE LID
AND SHAKE TO DISTRIBUTE THE ALGAE EVENLY**

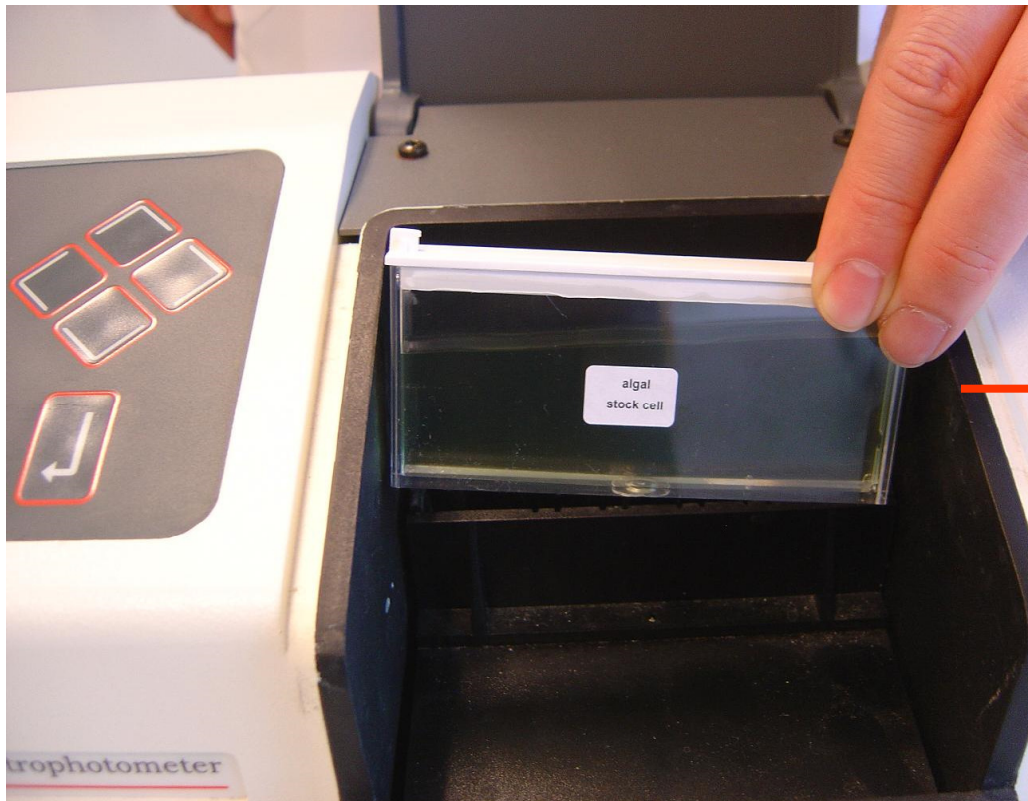

21

PUT THE ALGAL STOCK CELL IN THE SPECTROPHOTOMETER
AND READ THE OPTICAL DENSITY (OD₁) AFTER 10 SECONDS

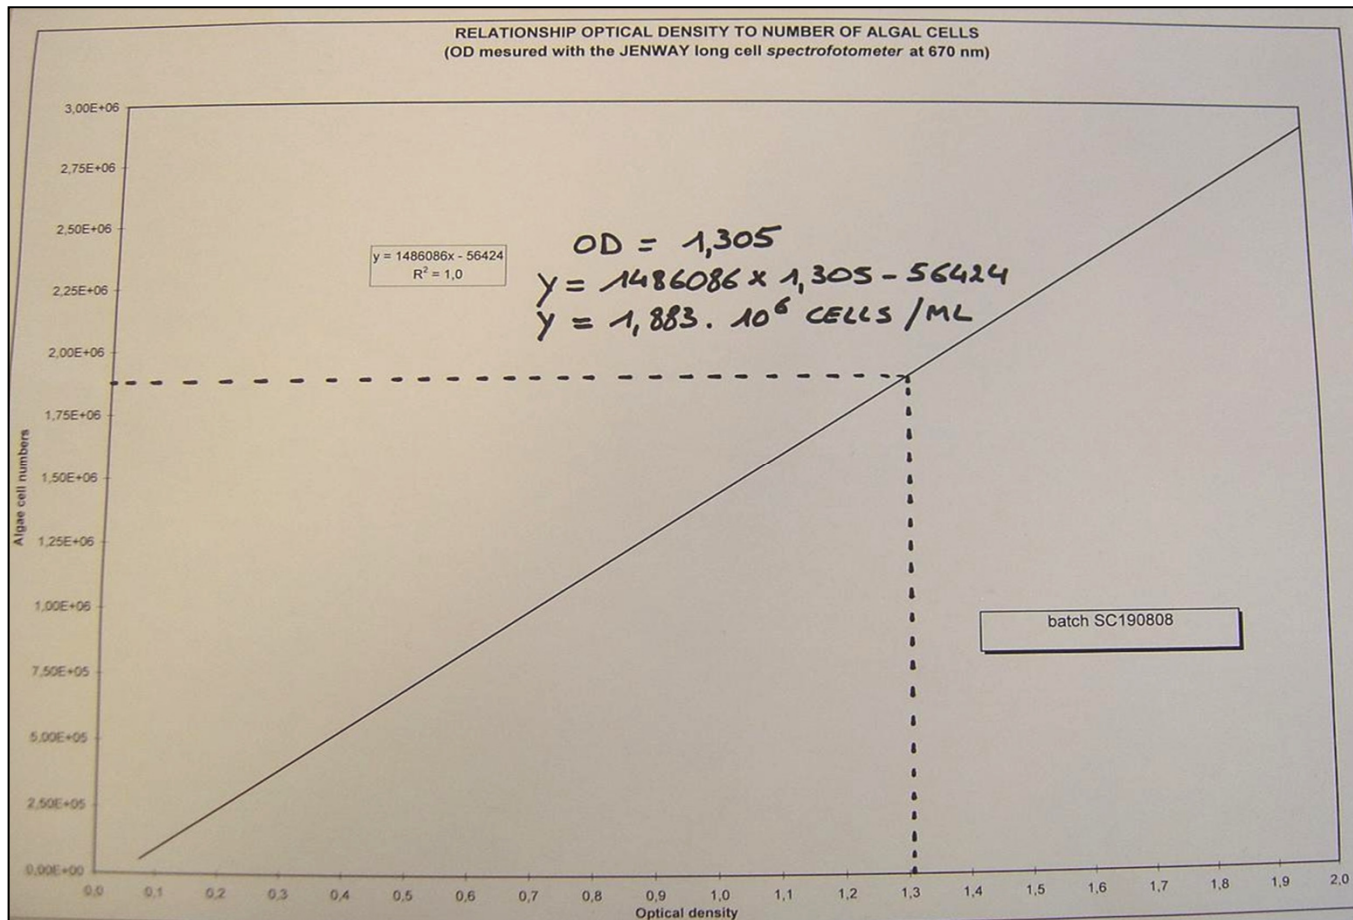



- TAKE THE OD/N SHEET
(optical density/algal number)

- WITH THE AID OF THE REGRESSION FORMULA CALCULATE THE NUMBER OF ALGAE N1 CORRESPONDING TO THE MEASURED OD1 IN THE ALGAL STOCK CELL
- WITH $N2 = 1.10^6$ ALGAE/ML, CALCULATE FROM THE $N1/N2$ RATIO THE DILUTION FACTOR NEEDED TO REACH OD2 (corresponding to 1.10^6 algae/ml)

23

**POUR THE 25 ML ALGAL
SUSPENSION FROM THE
ALGAL STOCK CELL INTO
A 100 ML FLASK**

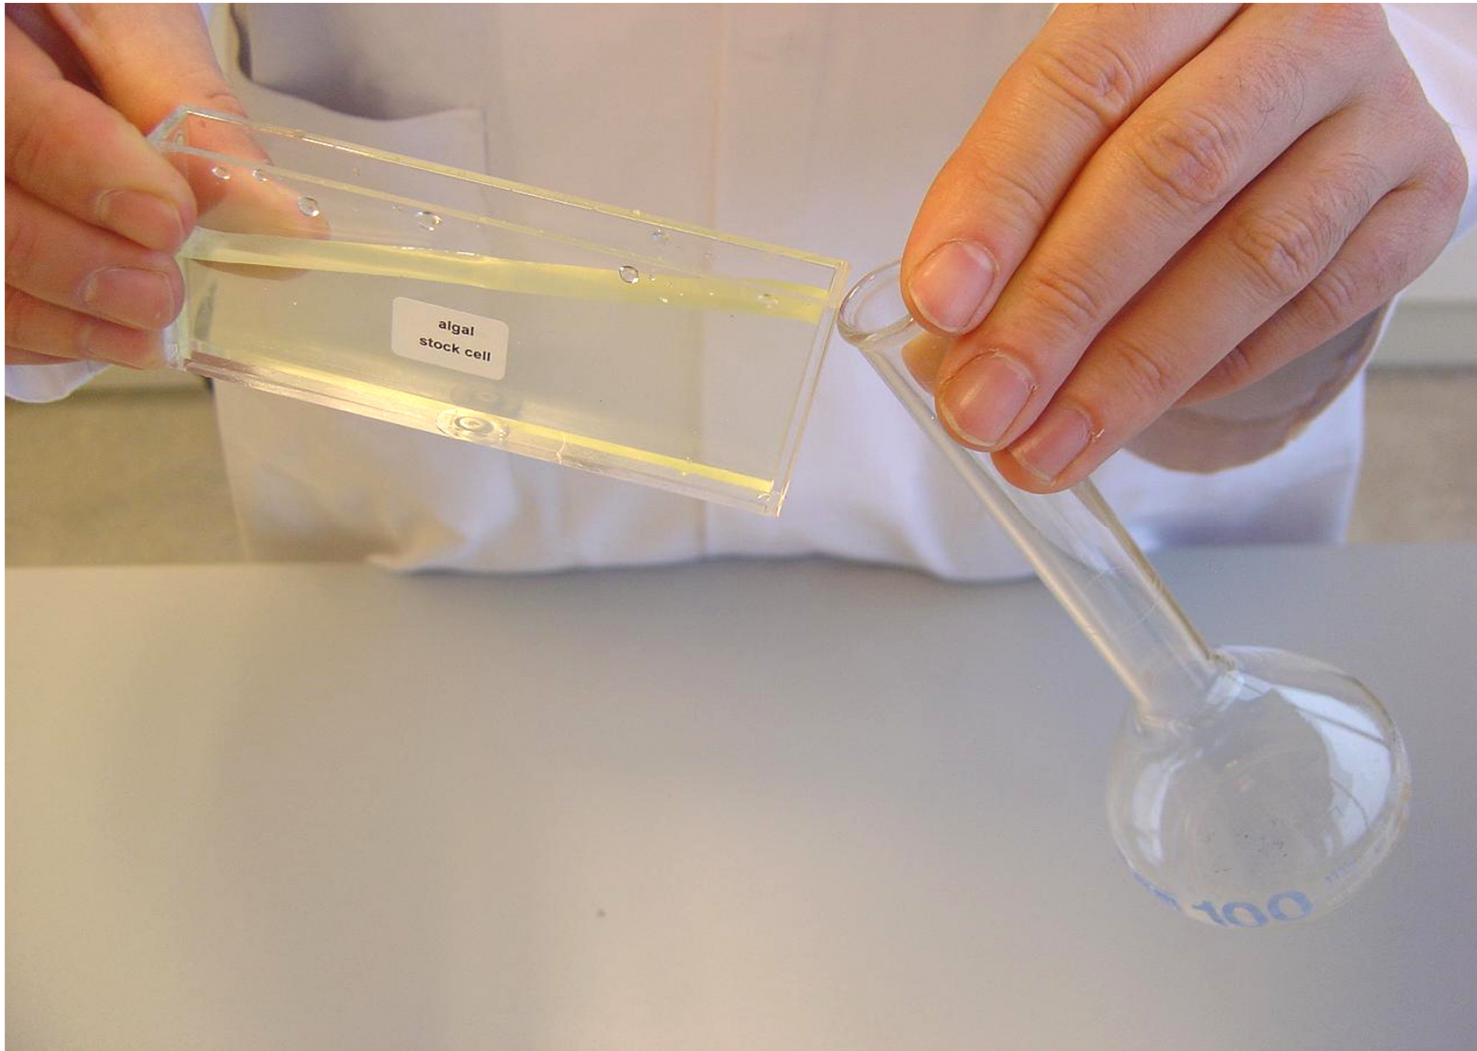

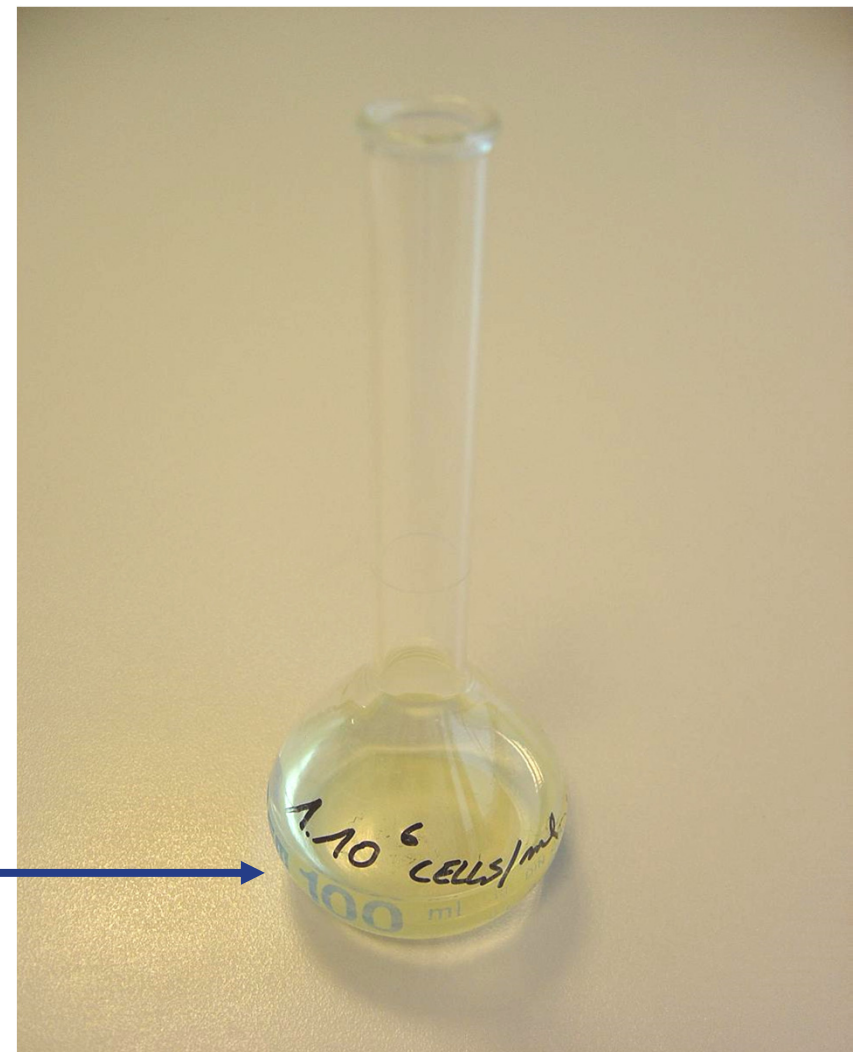


24

ADD THE CALCULATED VOLUME OF ALGAL CULTURING MEDIUM
TO THE FLASK, TO MAKE UP A SUSPENSION OF 1.10^6 ALGAL CELLS / ML

25


PREPARATION OF THE TOXICANT DILUTION SERIES


TAKE SIX 200 ML CALIBRATED
FLASKS AND LABEL THEM FROM
C0 TO C5

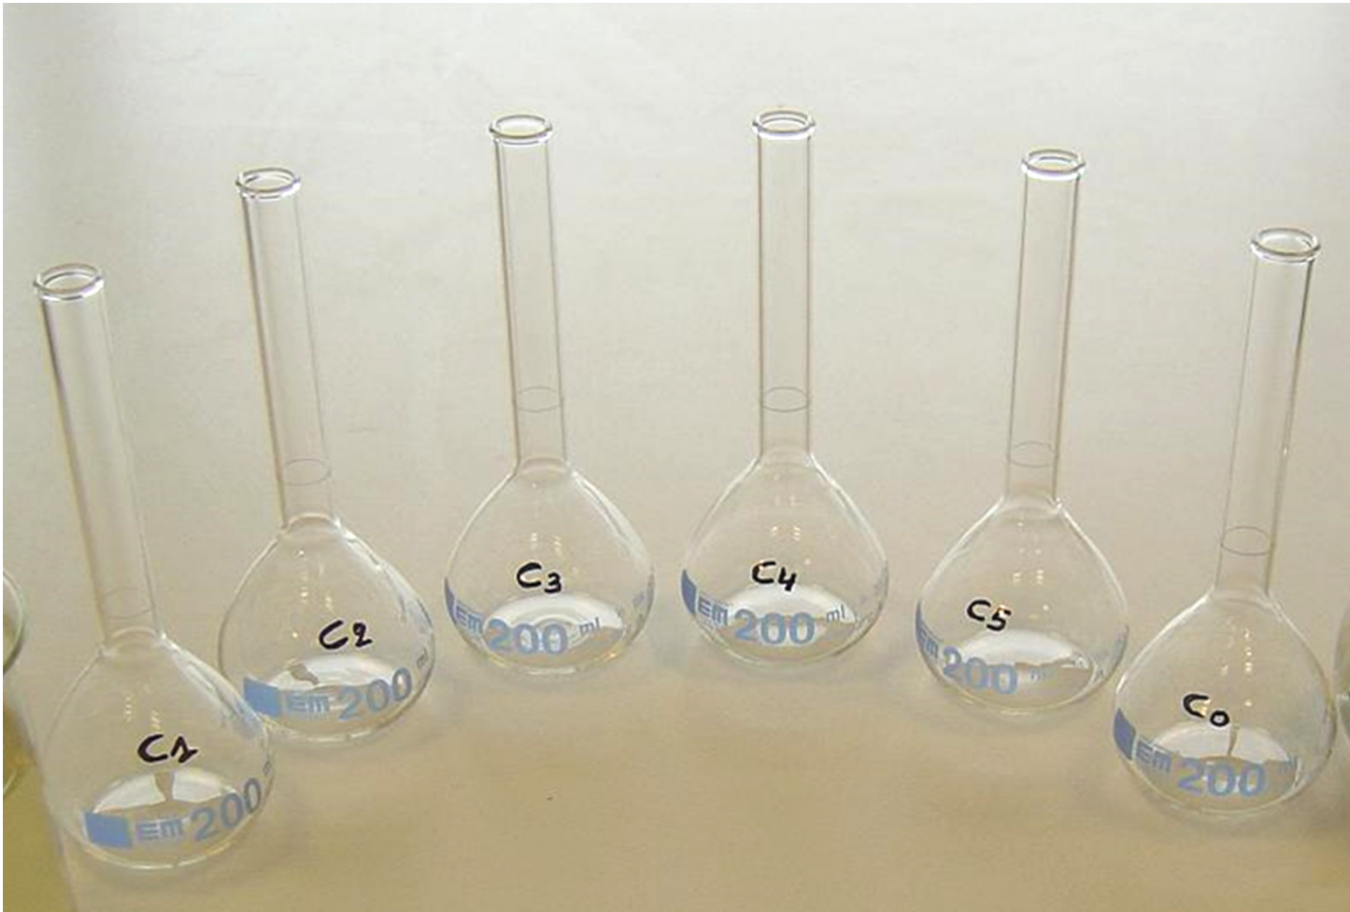

26

TO ELIMINATE TURBIDITY,
SAMPLES MUST BE
FILTERED BEFORE TESTING
(e.g. over a membrane filter
of 0.45 μm),

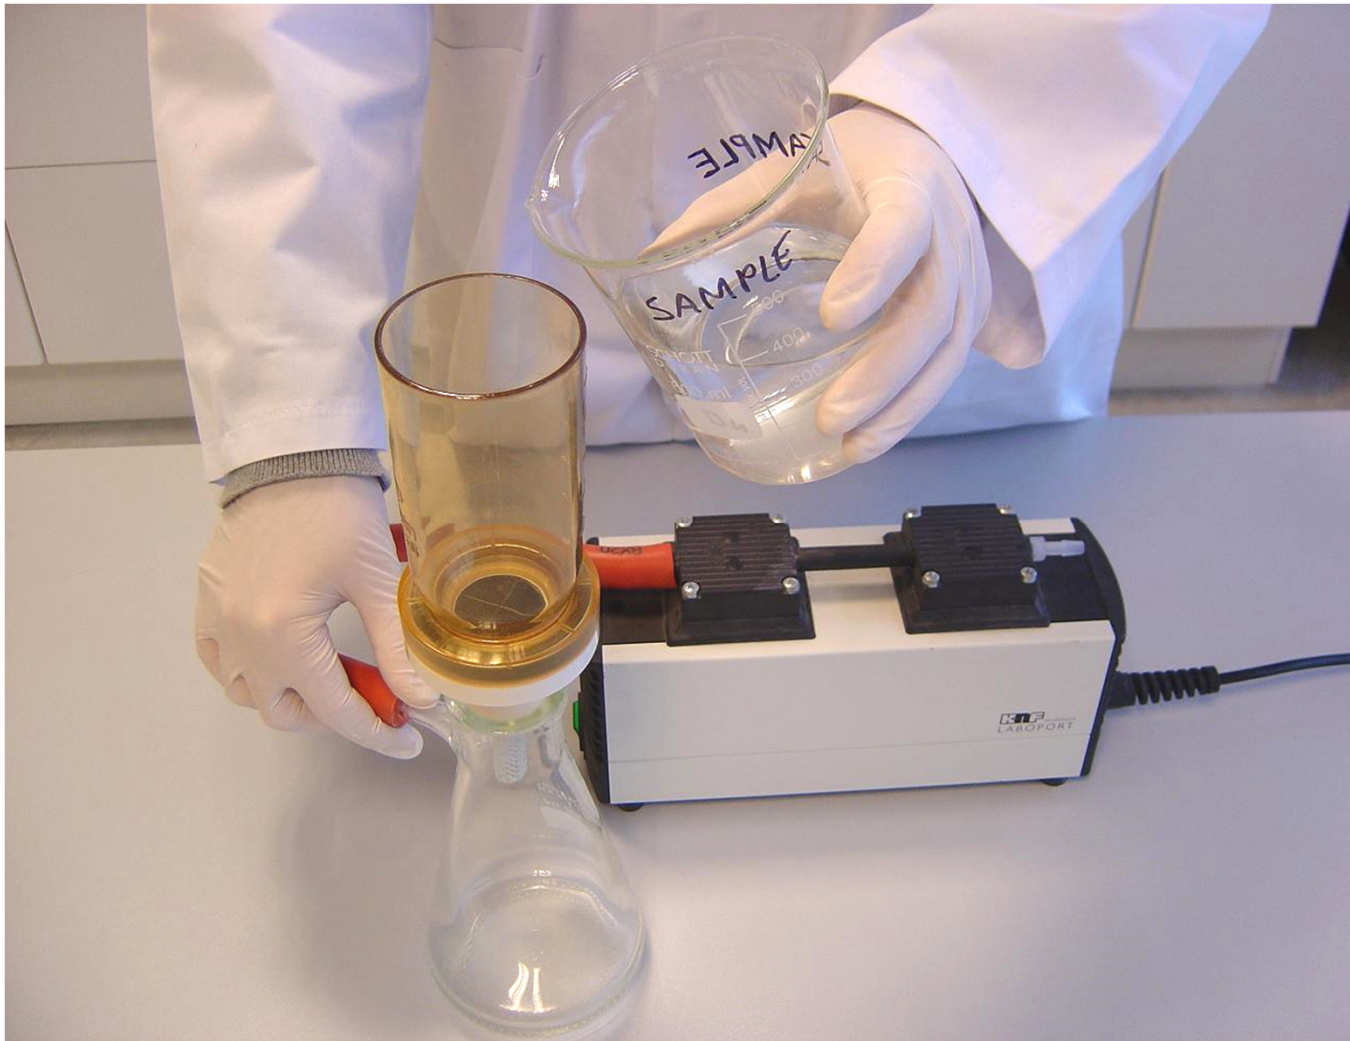

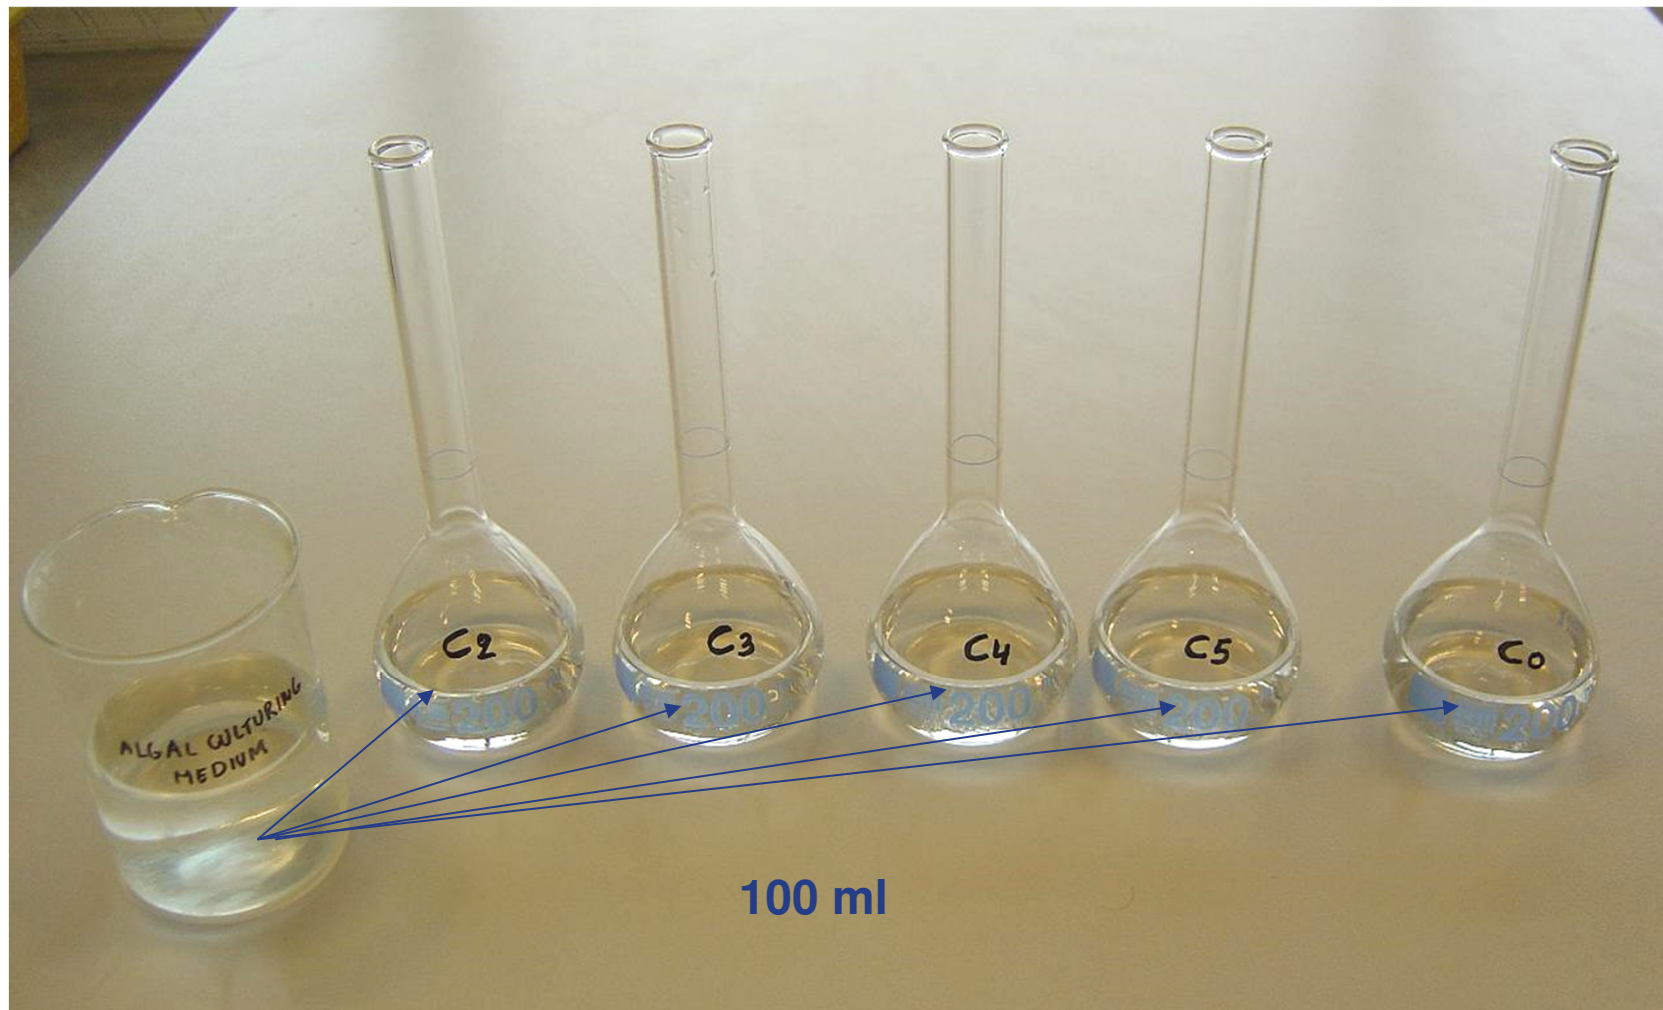


27

PUT 100 ML ALGAL CULTURING MEDIUM
IN THE 200 ML FLASKS C0, C2, C3, C4 AND C5

28



**FILL FLASK C1
TO THE 200 ML MARK
WITH THE FILTERED SAMPLE**

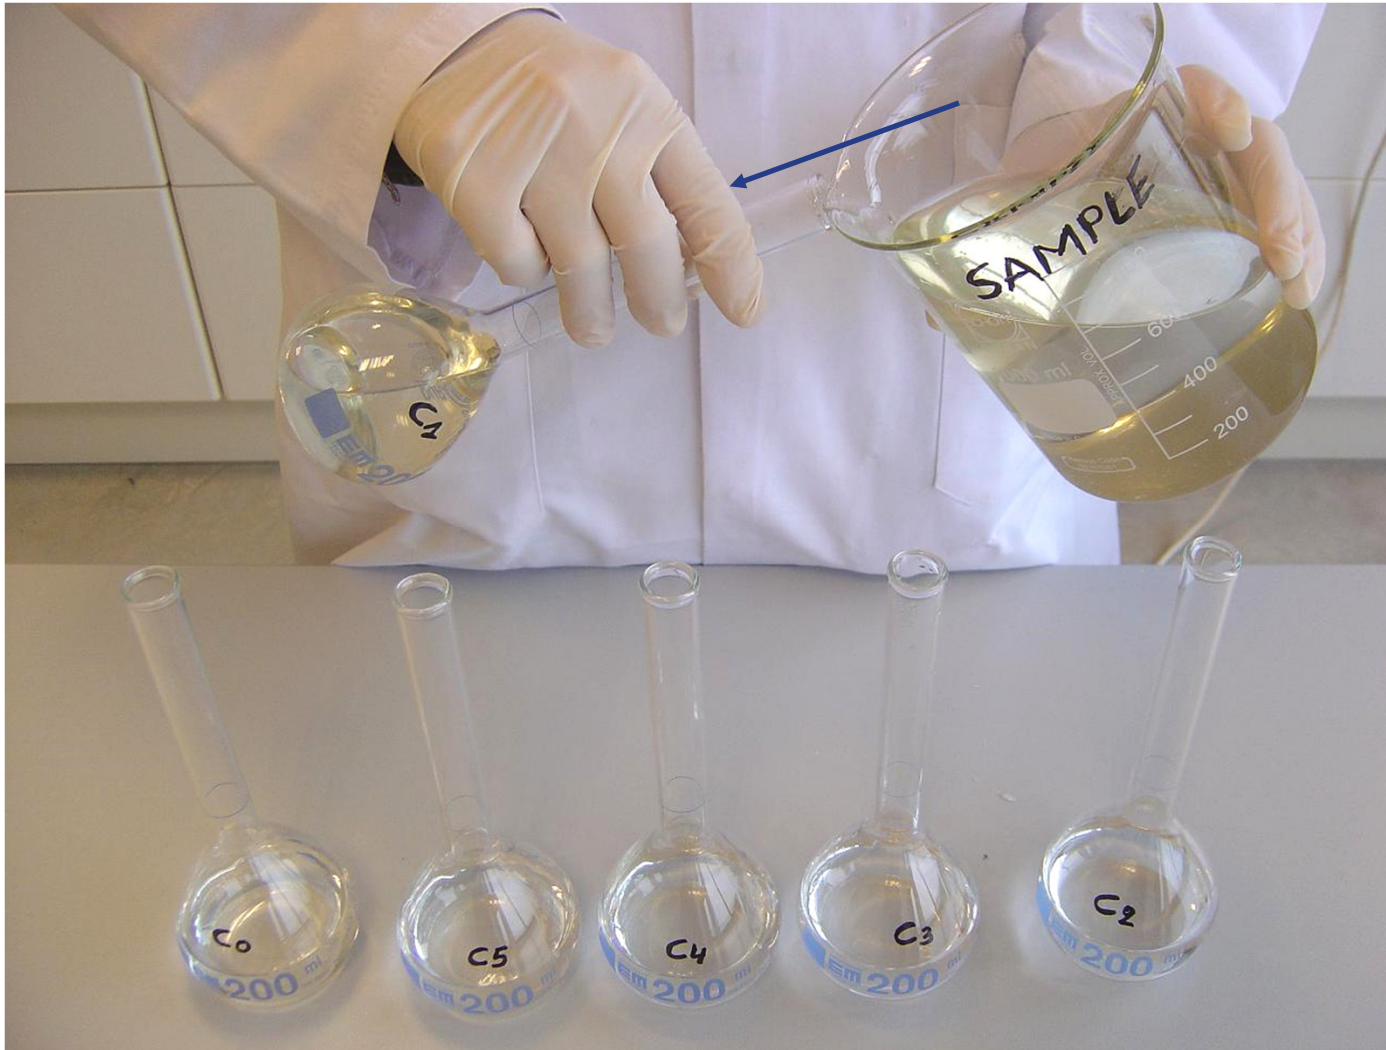



29

- ADD 2 ML “NUTRIENT STOCK SOLUTION A” AND 0.2 ML OF NUTRIENT STOCK SOLUTIONS B, C AND D TO FLASK C1
- STOPPER THE FLASK AND SHAKE TO MIX THE CONTENTS

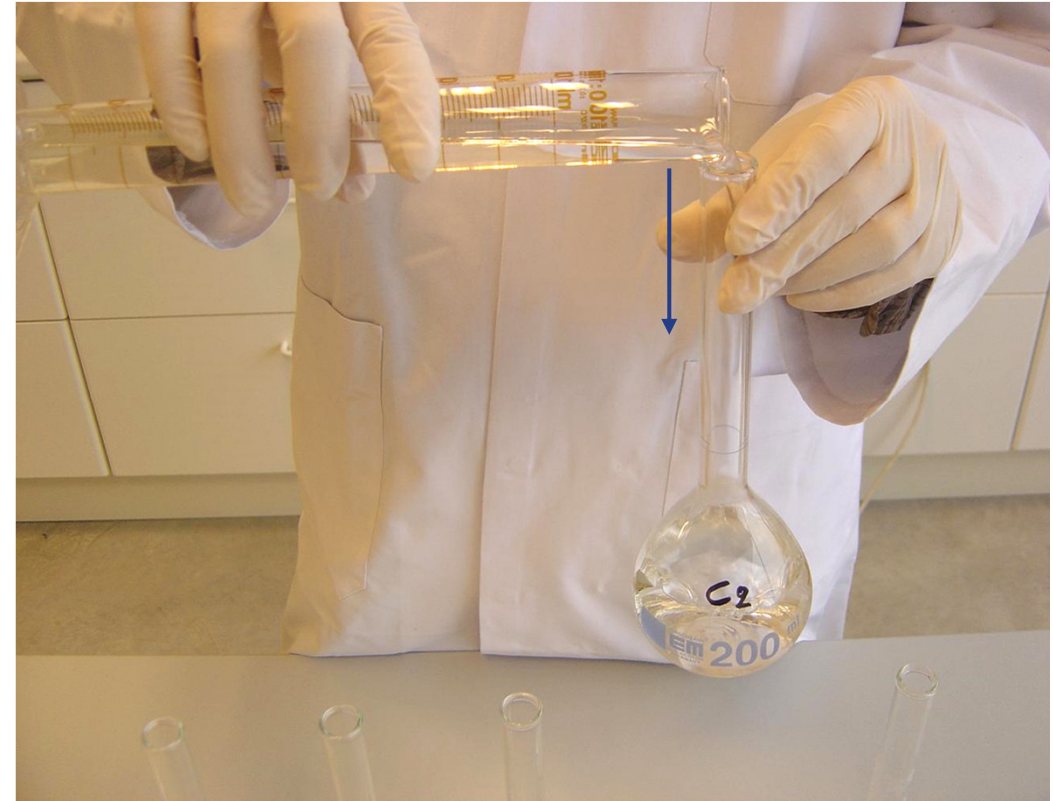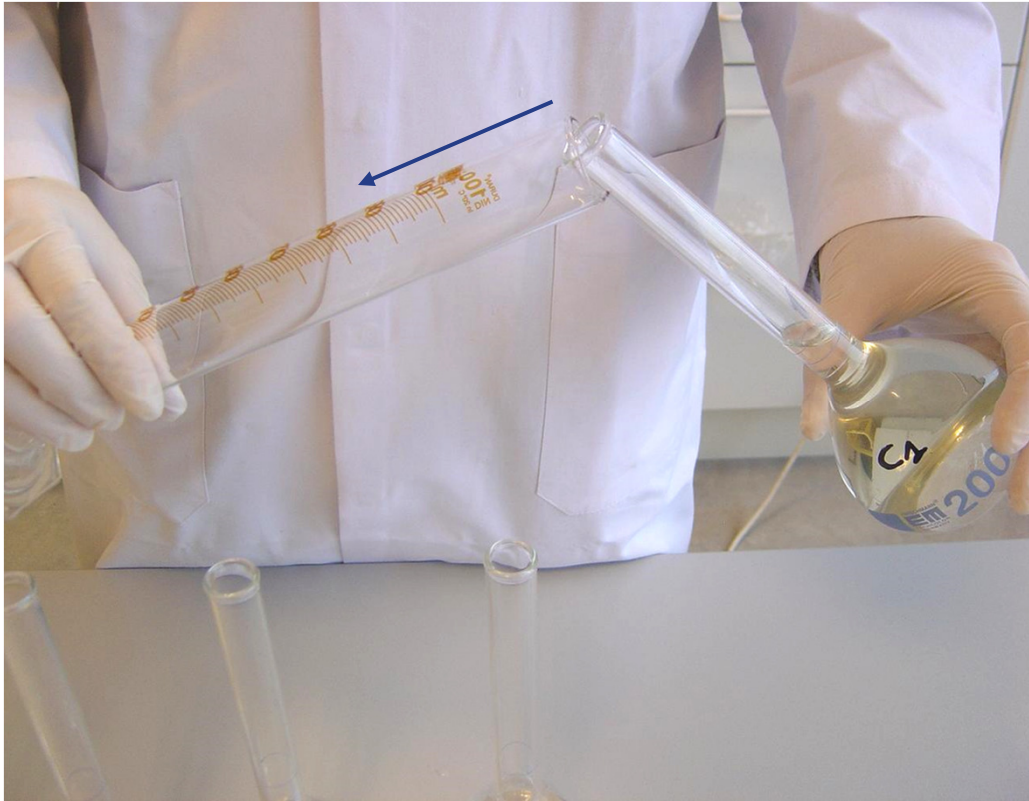


30

- POUR 100 ML SAMPLE FROM FLASK C1 INTO A GRADUATED CYLINDER AND TRANSFER THIS VOLUME INTO FLASK C2 TO MAKE THE FIRST 1:1 DILUTION
- STOPPER FLASK C2 AND SHAKE TO HOMOGENIZE THE CONTENTS


31

REPEAT THE FORMER
DILUTION PROCEDURE
FOR THE OTHER FLASKS
(i.e.. 100 ml from C2 to C3, etc.)

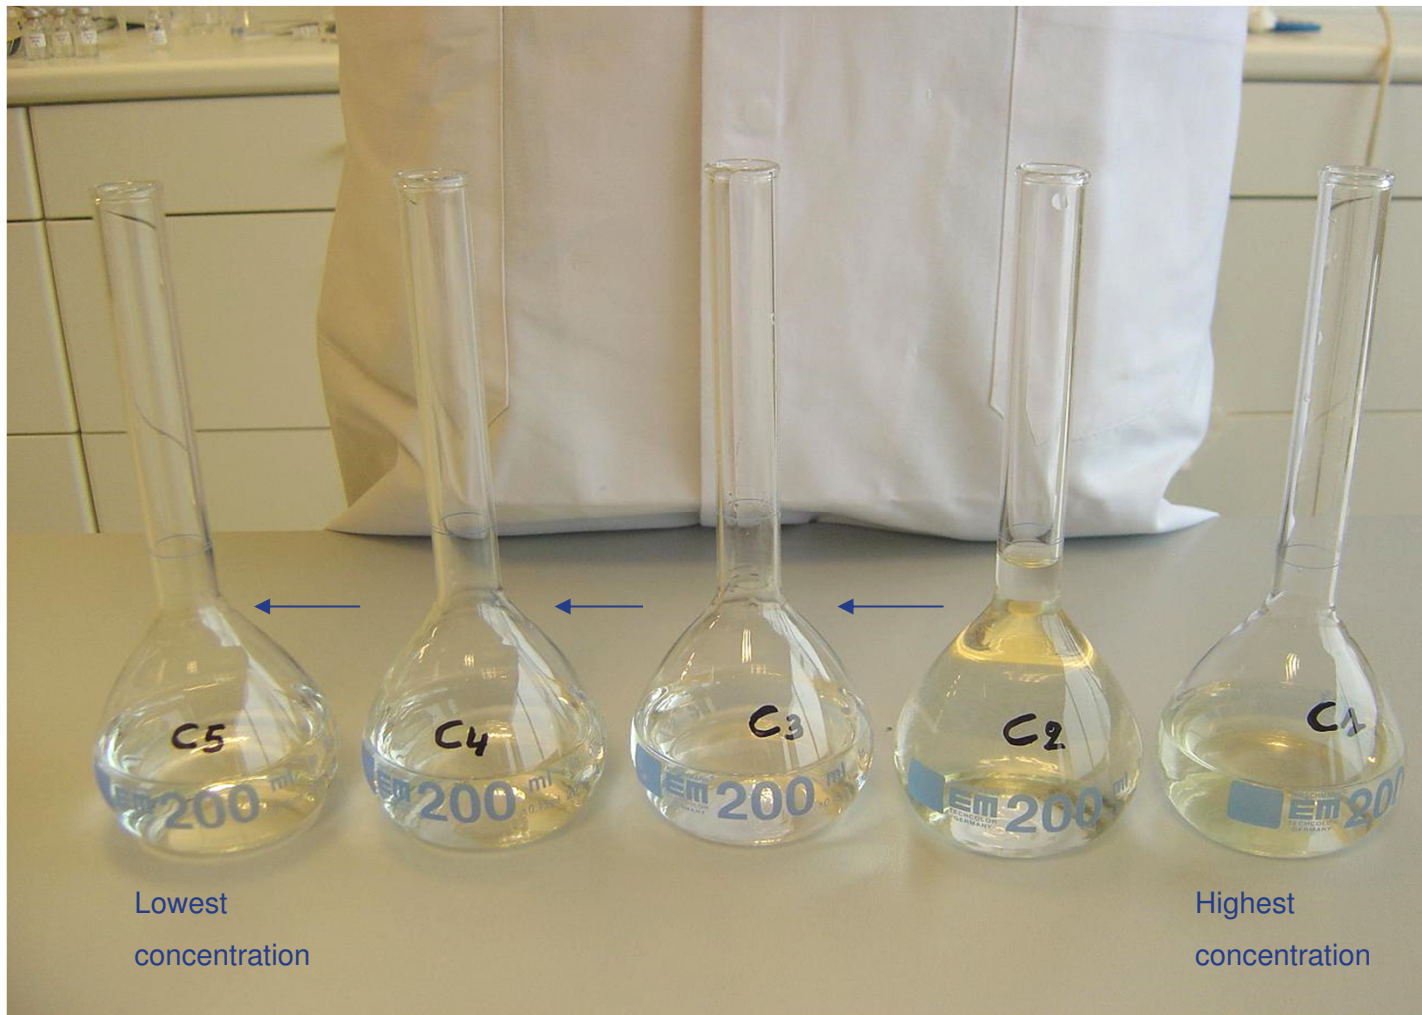

32


REMOVE AND DISCARD
100 ML SOLUTION FROM
FLASK C5 TO HAVE 100 ML
SOLUTIONS IN EACH FLASK

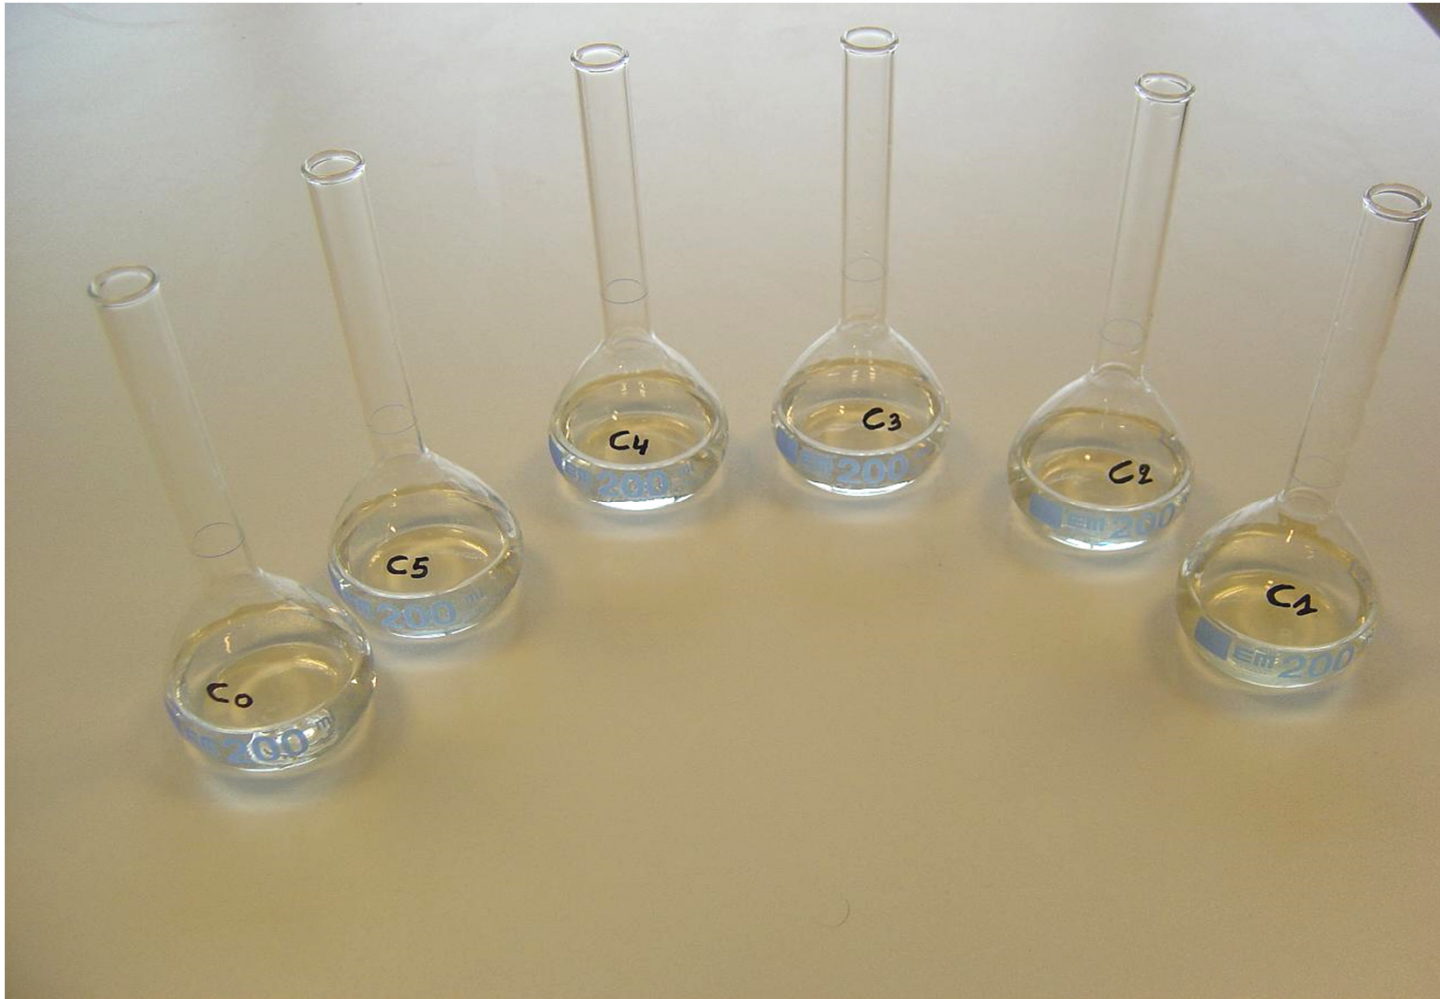




33

- TAKE THE FLASK CONTAINING THE $1.10^6/\text{ML}$ ALGAL SUSPENSION AND SHAKE IT GENTLY
- ADD 1 ML ALGAL SUSPENSION TO EACH OF THE 6 FLASKS C0 TO C5, IN ORDER TO OBTAIN AN INITIAL ALGAL CONCENTRATION OF 1.10^4 CELLS/ML IN EACH FLASK

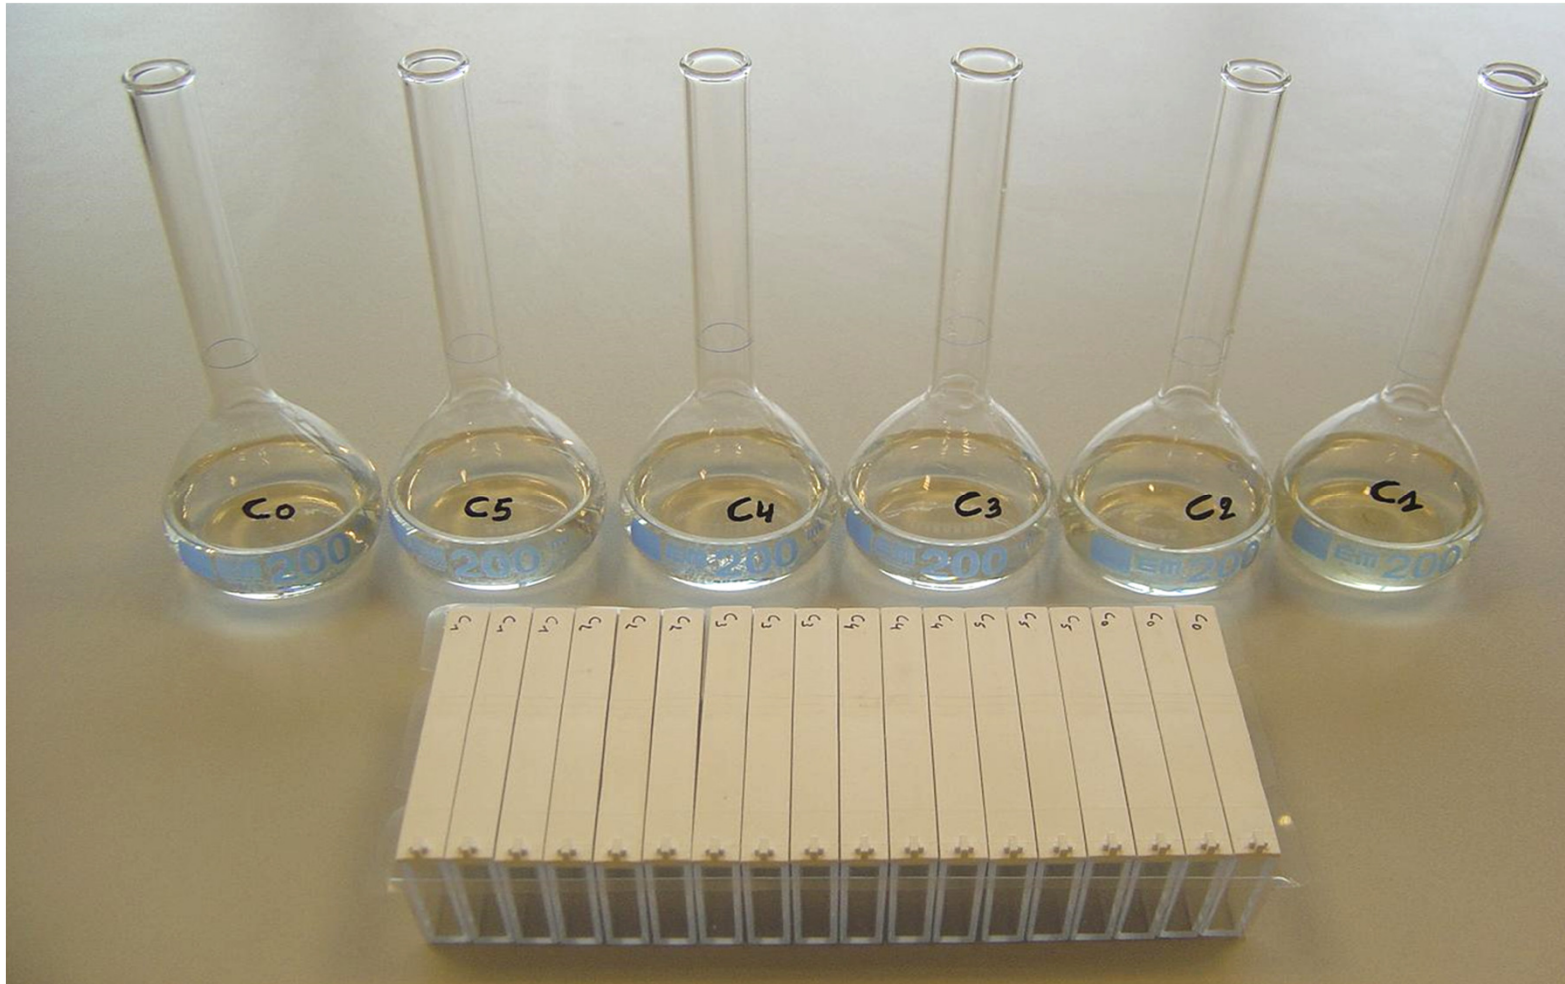

34

**TRANSFER OF THE ALGAE-TOXICANT DILUTIONS
INTO THE TEST VIALS**

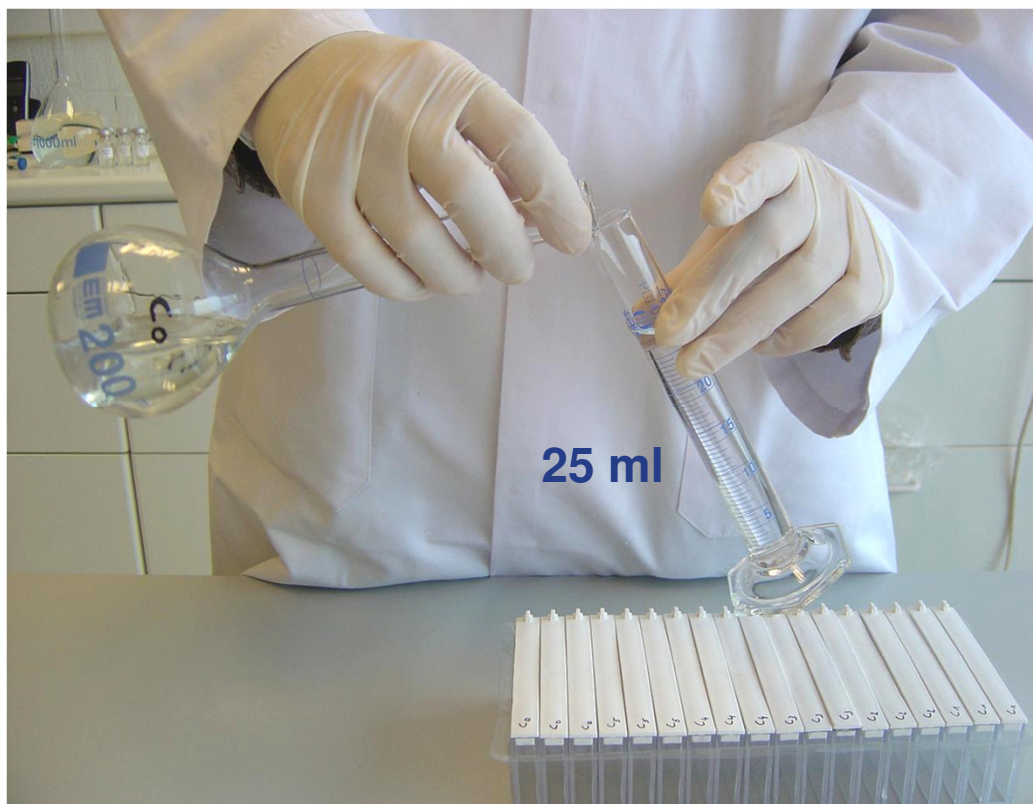


35

- LABEL ALL THE LONG CELLS ON THEIR LID (3 replicates per dilution)
- AFTER THOROUGH SHAKING, TRANSFER 25 ML ALGAE-TOXICANT DILUTION FROM EACH FLASK INTO A GRADUATED CYLINDER, FOR FURTHER TRANSFER INTO THE CORRESPONDING LONG CELL (3 replicates per toxicant dilution)



36


- REDISTRIBUTE THE LONG CELLS IN THE HOLDING TRAY IN A RANDOM WAY
- LIFT UP THE LIDS OF THE CELLS A LITTLE AT ONE SIDE, AND SLIDE THE PLASTIC STRIP OVER THE OPEN PART OF THE LONG CELLS TO KEEP THEM SLIGHTLY OPEN DURING THE INCUBATION PERIOD

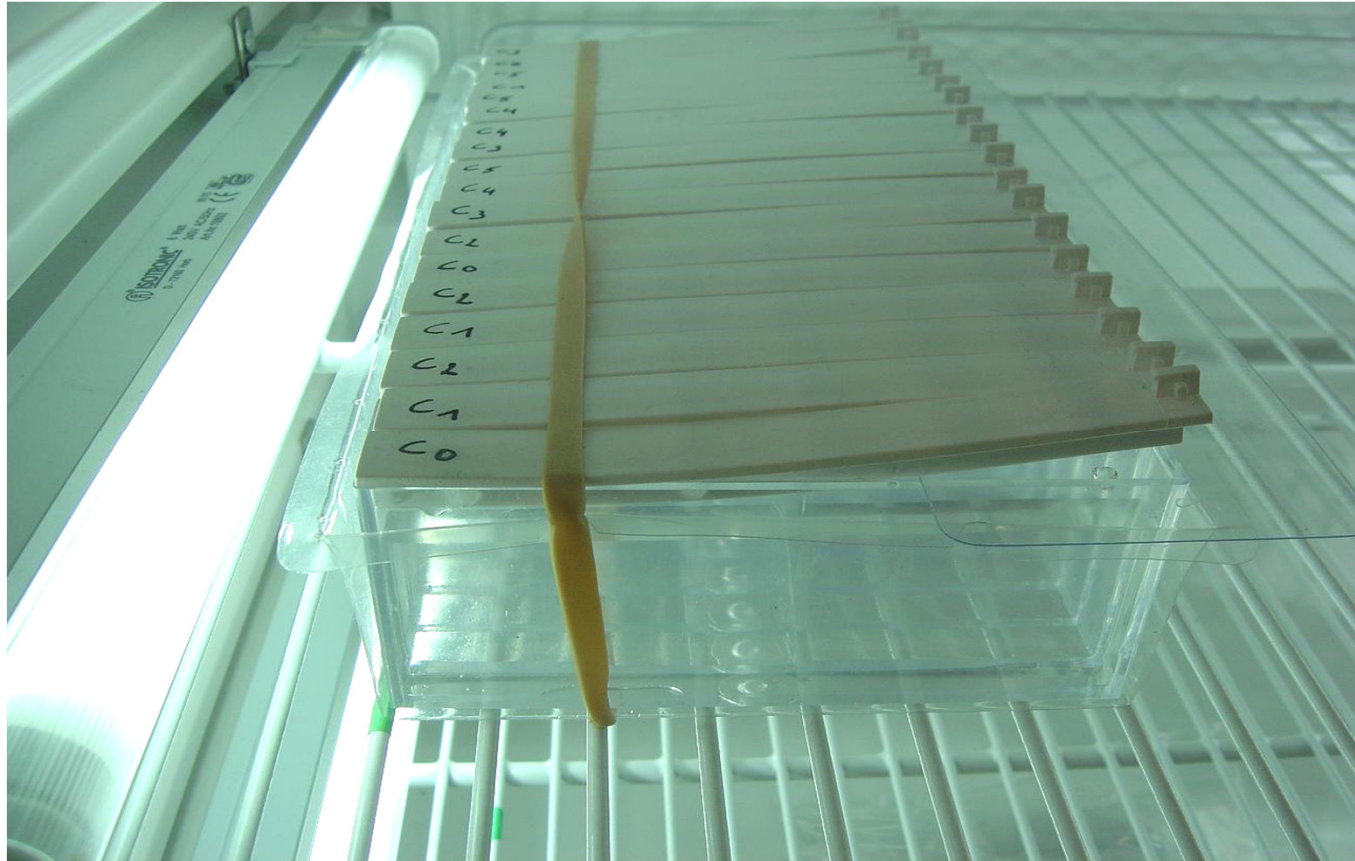

37

**INCUBATE THE HOLDING TRAY WITH THE LONG CELLS FOR 72h IN AN INCUBATOR
AT 23°C ± 2 °C, WITH CONTINUOUS ILLUMINATION:**

- SIDEWAY ILLUMINATION = 10000 LUX
- OR BOTTOM ILLUMINATION = 3000-4000 LUX

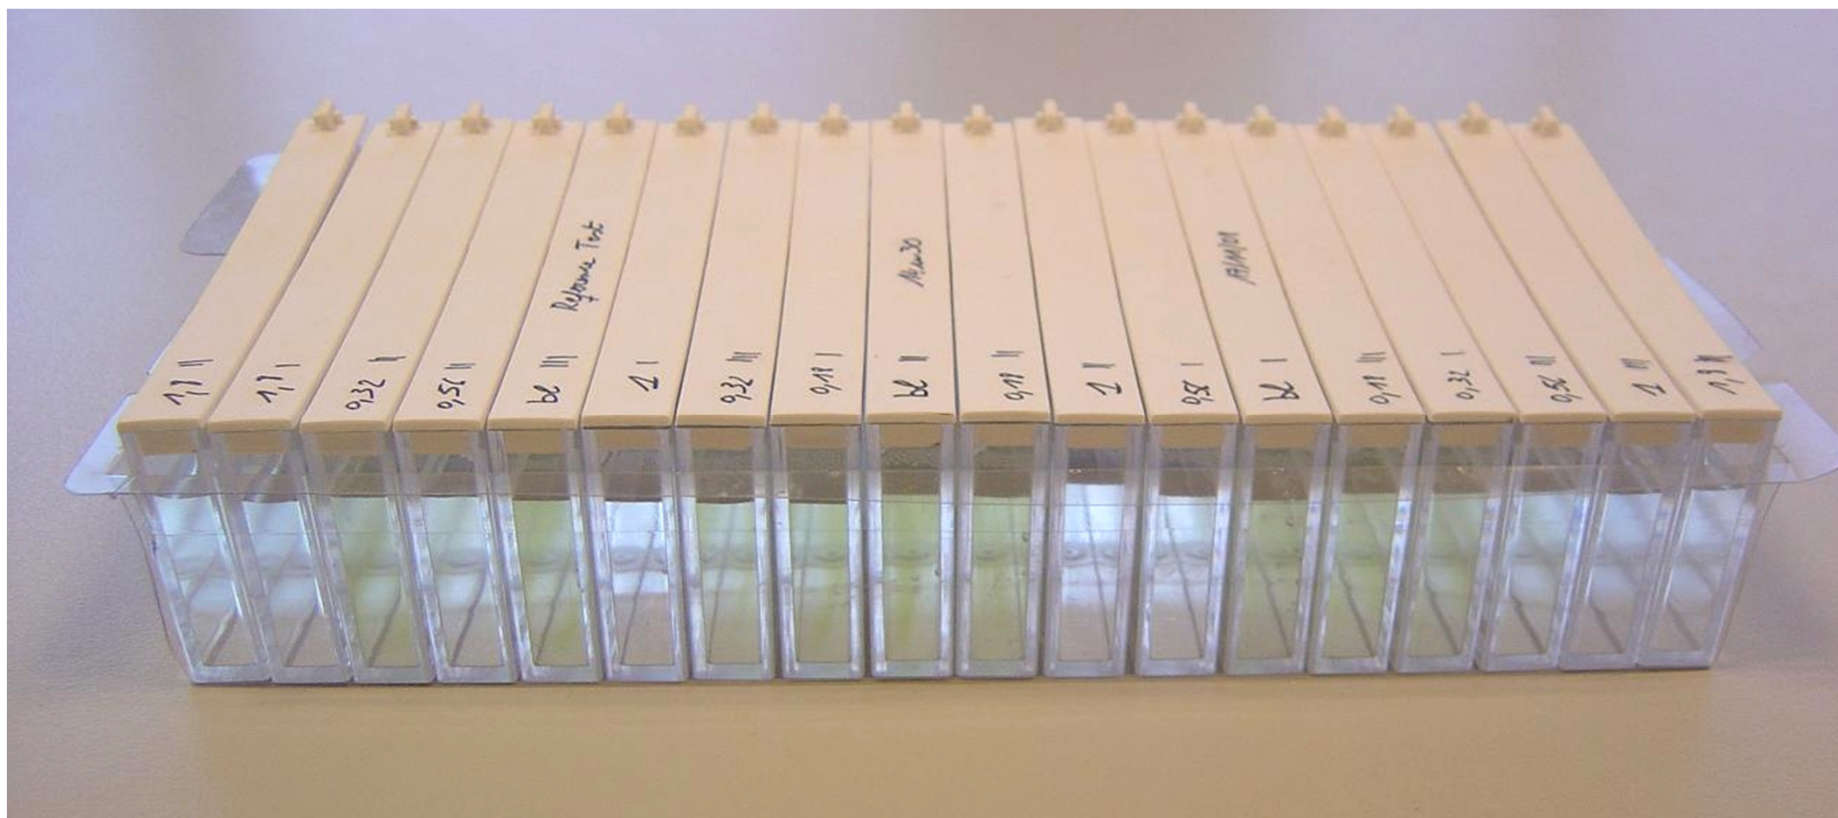

38


SCORING OF THE RESULTS

THE OD OF THE ALGAL SUSPENSIONS SHALL BE MEASURED EACH DAY DURING THE 3 DAYS OF THE TEST, I.E. AFTER 24h, 48h AND 72h EXPOSURE TO THE TOXICANT

39


**ZERO-CALIBRATE THE
SPECTROPHOTOMETER
PRIOR TO THE DAILY MEASUREMENT
OF THE OD IN THE LONG CELLS,**



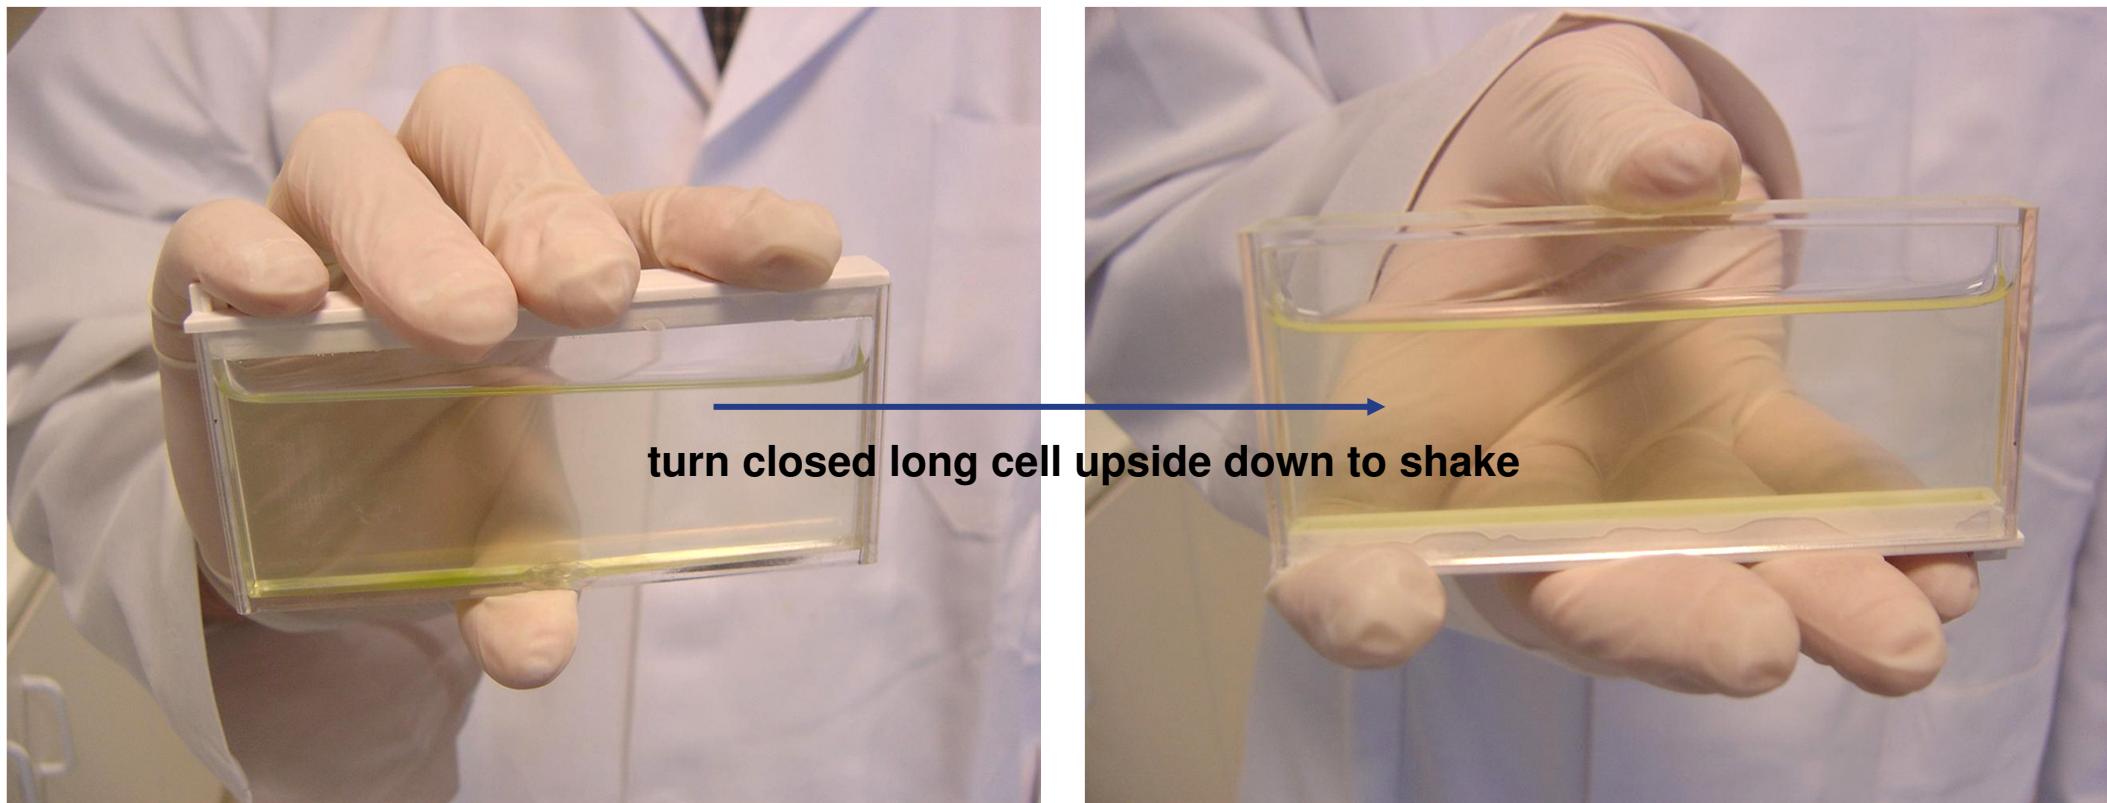

40

**IMMEDIATELY BEFORE MEASURING THE OD IN A LONG CELL, CLOSE THE CELL,
TURN IT UPSIDE DOWN AND SHAKE GENTLY TO RESUSPEND THE ALGAE EVENLY**

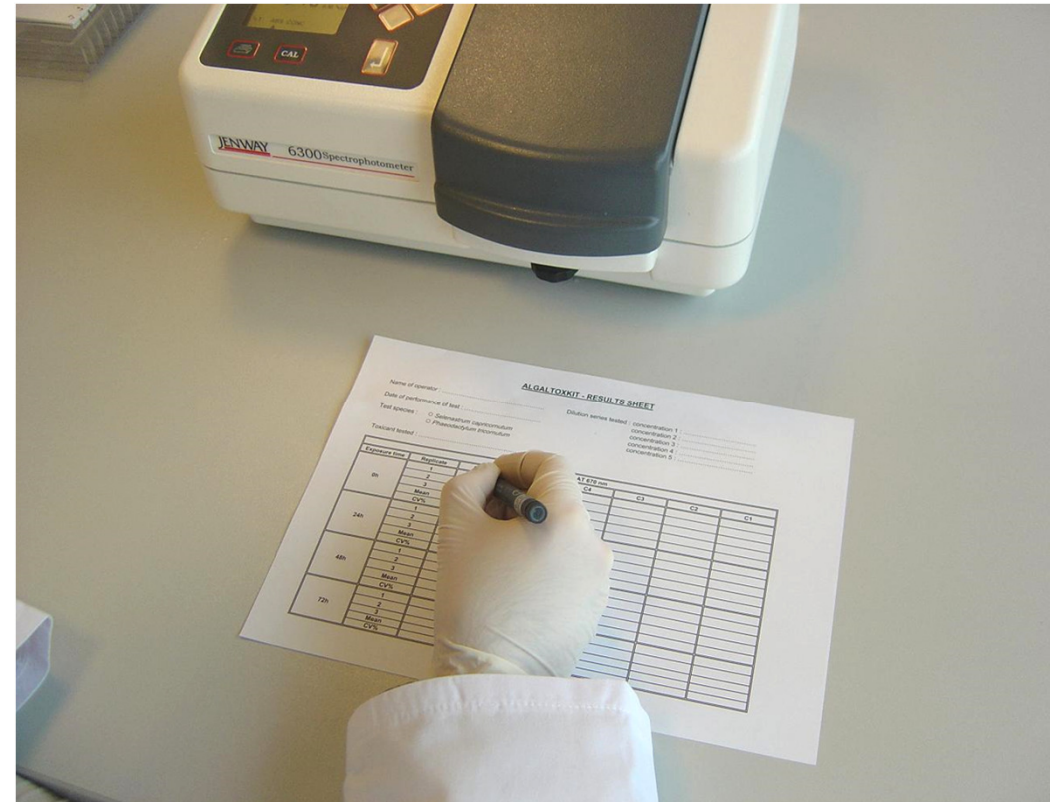

41

- SCORE THE DAILY OD RESULT OF EACH LONG CELL ON THE “RESULTS SHEET”
- PERFORM THE DATA TREATMENT OF THE RESULTS WITH AN APPROPRIATE PROGRAMME